


Journal Pre-proof

European Society for Vascular Surgery (ESVS) 2023 Clinical Practice Guidelines on Radiation Safety

Writing Committee, ESVS Guidelines Committee, Document Reviewers

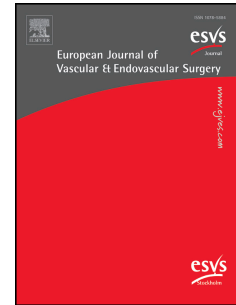

PII: S1078-5884(22)00546-9

DOI: <https://doi.org/10.1016/j.ejvs.2022.09.005>

Reference: YEJVS 8533

To appear in: *European Journal of Vascular & Endovascular Surgery*

Received Date: 19 August 2022

Accepted Date: 15 September 2022

Please cite this article as: Writing Committee, ESVS Guidelines Committee, Document Reviewers, European Society for Vascular Surgery (ESVS) 2023 Clinical Practice Guidelines on Radiation Safety, *European Journal of Vascular & Endovascular Surgery*, <https://doi.org/10.1016/j.ejvs.2022.09.005>.

This is a PDF file of an article that has undergone enhancements after acceptance, such as the addition of a cover page and metadata, and formatting for readability, but it is not yet the definitive version of record. This version will undergo additional copyediting, typesetting and review before it is published in its final form, but we are providing this version to give early visibility of the article. Please note that, during the production process, errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

© 2022 The Author(s). Published by Elsevier B.V. on behalf of European Society for Vascular Surgery.

European Society for Vascular Surgery (ESVS) 2023 Clinical Practice Guidelines on Radiation Safety

Bijan Modarai ^{a*}, Stéphan Haulon ^a, Elizabeth Ainsbury ^a, Dittmar Böckler ^a, Eliseo Vano-Carruana ^a, Joseph Dawson ^a, Mark Farber ^a, Isabelle Van Herzele ^a, Adrien Hertault ^a, Joost van Herwaarden ^a, Ashish Patel ^a, Anders Wanhainen ^a, Salome Weiss ^a

ESVS Guidelines Committee ^b: Frederico Bastos Gonçalves, Martin Björck, Nabil Chakfé, Gert J. de Borst, Raphaël Coscas, Nuno V. Dias, Florian Dick, Robert J. Hinchliffe, Stavros K. Kakkos, Igor B. Koncar, Philippe Kolh, Jes S. Lindholt, Santi Trimarchi, Riikka Tulamo, Christopher P. Twine, Frank Vermassen

Document Reviewers ^c: Klaus Bacher, Elias Broutzos, Fabrizio Fanelli, Liliana A. Fidalgo Domingos, Mauro Gargiulo, Kevin Mani, Tara M. Mastracci, Blandine Maurel, Robert A. Morgan, Peter Schneider

For a full list of the authors' affiliations, please refer to Appendix

^a **Guideline Writing Committee:** Bijan Modarai (London, United Kingdom, chair), Stéphan Haulon (Paris, France, co-chair), Adrien Hertault (Villeneuve d'Ascq, France), Anders Wanhainen (Uppsala, Sweden), Ashish Patel (London, United Kingdom), Dittmar Böckler (Heidelberg, Germany), Eliseo Vano (Madrid, Spain), Elizabeth Ainsbury (London, United Kingdom), Isabelle Van Herzele (Ghent, Belgium), Joost van Herwaarden (Utrecht, The Netherlands), Joseph Dawson (South Australia, Australia), Mark Farber (Chapel Hill, NC, USA), Salome Weiss (Bern, Switzerland)

^b **ESVS Guidelines Committee:** Frederico Bastos Gonçalves (Lisbon, Portugal), Martin Björck (Uppsala, Sweden), Nabil Chakfé (Strasbourg, France), Gert J. de Borst, (Utrecht, The Netherlands), Raphaël Coscas (Versailles, France), Nuno V. Dias (Malmö, Sweden), Florian Dick (Berne, Switzerland), Robert J. Hinchliffe (Bristol, United Kingdom), Stavros K. Kakkos (Patras, Greece), Igor B. Koncar (Belgrade, Serbia), Philippe Kolh (Liège, Belgium), Jes S. Lindholt (Odense, Denmark), Santi Trimarchi (Milan, Italy), Riikka Tulamo (Helsinki, Finland), Christopher P. Twine (Bristol, United Kingdom), Frank Vermassen (Ghent, Belgium, review coordinator)

^c **Document Reviewers:** Klaus Bacher (Ghent, Belgium), Elias Broutzos (Athens, Greece), Fabrizio Fanelli (Florence, Italy), Liliana A. Fidalgo Domingos (Faro, Portugal), Mauro Gargiulo (Bologna, Italy), Kevin Mani (Uppsala, Sweden), Tara M. Mastracci (London, United Kingdom), Blandine Maurel (Nantes, France), Robert A. Morgan (London, United Kingdom), Peter Schneider (San Francisco, CA, USA)

*Corresponding author: Bijan Modarai Academic Department of Vascular Surgery, School of Cardiovascular and Metabolic Medicine and Sciences, BHF Centre of Excellence and the Biomedical Research Centre at Guy's & St Thomas' NHS Foundation Trust and King's College London, United Kingdom (chair)

TABLE OF CONTENTS

40	GLOSSARY	8
41	LIST OF ABBREVIATIONS	13
42	Chapter 1. Introduction and general aspects	16
43	1.1 The need for radiation protection guidelines	16
44	1.2 Methodology	17
45	1.2.1. Strategy	17
46	1.2.2. Literature search and selection	17
47	1.2.3. Weighing the evidence	18
48	1.2.4. Contributors to the guideline	20
49	1.3 The patient and public perspective	20
50	1.3.1 Background and aims	20
51	1.3.2 Feedback from stakeholders	22
52	1.3.3 Responsibilities of the endovascular operator to justify and explain radiation exposure to	
53	patients.....	23
54	1.4 Plain language summary	26
55	Chapter 2. Measuring radiation exposure and the associated risks of exposure	27
56	2.1 Radiation exposure during Xray guided procedures	27
57	2.2 Dosimetric parameters	27
58	2.2.1 Direct Dose parameters:	27
59	2.2.2 Indirect Dose parameters:.....	28

60	2.3 Existing literature informing radiation exposure during endovascular procedures	30
61	2.4 Diagnostic reference levels	36
62	2.5 Biological risk related to radiation exposure.....	38
63	2.5.1 Stochastic and Deterministic Effects of Radiation Exposure.....	38
64	2.5.1.1 Estimators of stochastic risks	39
65	2.5.1.2 Estimators of deterministic risks	40
66	2.5.2 The biological response to radiation exposure	43
67	2.5.3 Biomarkers of radiation exposure	43
68	2.5.4 Risks associated with occupational radiation exposure to patients	44
69	2.5.5 Risks associated with occupational radiation exposure to operators.....	46
70	Chapter 3. Legislation regarding exposure limits for radiation exposed workers	48
71	3.1 Framework for radiation safety legislation	48
72	3.2 Current legislation defining safe radiation exposure limits	49
73	3.3 Pregnancy and radiation exposure.....	53
74	Chapter 4. Measuring, monitoring and reporting occupational radiation exposure.....	55
75	4.1 Background and Introduction.....	55
76	4.2. Monitoring radiation exposure during endovascular interventions	55
77	4.3 Personal radiation exposure monitoring devices.....	57
78	4.4 Monitoring and reporting occupational radiation doses	59
79	4.5 Inaccuracy and uncertainty associated with personal dosimetry.....	60
80	Chapter 5. Radiation safety practice in the endovascular operating room	61
81	5.1 The “As Low As Reasonably Achievable” (ALARA) principle	61

82	5.2 Minimising radiation emitted by the C arm	64
83	5.3 Low Dose Settings	64
84	5.3.1 Fluoroscopy Time and Last Image Hold.....	64
85	5.3.2 Dose Settings & Automatic Brightness Control.....	65
86	5.3.3 Fluoroscopy and Pulse Rate	66
87	5.4 Collimation	69
88	5.5 Anti-scatter Grid Removal	71
89	5.6 Dose Reduction Hardware and Software	72
90	5.6.1 Advanced Dose Reduction Hardware & Software.....	72
91	5.6.2 Pre-Operative Planning Software.....	72
92	5.6.3 3D Image Fusion Software.....	73
93	5.6.4 Detectors and image intensifiers	74
94	5.6.4.1 Image Intensifiers and Flat Panel Detectors.....	74
95	5.6.4.2 Optimal use of Flat Panel Detectors to minimise Radiation Dose	75
96	5.7 Magnification.....	76
97	5.7.1 Conventional Magnification	76
98	5.7.2 Digital Zoom	77
99	5.8 Dose reports from modern Xray machines	78
100	5.9 Maintenance	79
101	5.10 Endovascular operating rooms: Hybrid suites & interventional platforms	80
102	5.10.1 Mobile C Arms	80
103	5.10.2 Fixed C arms and Hybrid Suites	80

104	5.10.3 Operator Controlled Imaging Parameters.....	82
105	5.11 Positioning around the patient	83
106	5.11.1 Imaging Chain Geometry.....	83
107	5.11.2 Gantry Angulation	86
108	5.11.3 The Inverse Square Law and 'Stepping Away'	88
109	5.11.4 Positioning around the Table	89
110	Chapter 6. Radiation protection equipment in the endovascular operating room	92
111	6.1 Introduction.....	92
112	6.2 Personal protection devices	93
113	6.2.1 Wearable aprons	93
114	6.2.2 Thyroid Collar	96
115	6.2.3 Leg shields	97
116	6.2.4 Glasses and visors.....	97
117	6.2.5 Hand shields	99
118	6.2.6 Head shields	101
119	6.3 Other radiation shielding equipment.....	103
120	6.3.1 Suspended personal radiation protection systems.....	103
121	6.3.2 Radiation protective shielding above and below the table.....	106
122	6.3.3 Radiation protective patient drapes	109
123	Chapter 7. Education and training in radiation protection	112
124	7.1 Introduction.....	112
125	7.2 Delivery of radiation protection education and training	113

126	7.3 Theoretical courses	114
127	7.4 Practical training.....	115
128	7.5 Timing of radiation protection education and training.....	117
129	Chapter 8. Future technologies and gaps in evidence	120
130	8.1 New technologies.....	120
131	8.1.1 Three dimensional (3D) navigation	120
132	8.1.2 Robotic tracking.....	122
133	8.1.3 Artificial Intelligence.....	123
134	8.2 Gaps in practice and evidence.....	124
135	8.2.1..... Global harmonisation of radiation safety practices	
136	124
137	8.2.2..... Radiation dosage reference levels	
138	124
139	8.2.3..... Pregnant staff in the endovascular operating room	
140	125
141	8.2.4..... Biological correlates of radiation exposure	
142	125
143	8.2.5..... The value of real time dosimetry	
144	126
145	8.2.6..... Operator control of C arm equipment	
146	126
147	8.2.7..... Personal protection equipment	
148	127

149	8.2.8.....	Education and training
150	127
151	REFERENCES	129
152	APPENDICES.....	173
153	ACKNOWLEDGEMENTS	174
154		
155		
156		

GLOSSARY

Absorbed dose: The mean energy imparted to matter of mass by ionising radiation. The SI unit for absorbed dose is joule per kilogram and is usually denoted in Gray (Gy). Organ absorbed doses are often quoted.

Air kerma (AK): The quotient of the sum of the kinetic energies of all charged particles liberated by uncharged particles in a mass, dm , of air. The AK is measured or calculated at a reference point 15 cm from the isocentre in the direction of the focal spot cumulated from a whole Xray guided procedure.

Air-kerma area product (KAP, or Dose Area product, DAP): The KAP is the integral of the air kerma free in air (i.e. in the absence of backscatter) over the area of the Xray beam in a plane perpendicular to the beam axis (usually measured in Gy.cm²). The IRCP now recommends referring to those values as Air-Air-kerma area product (P_{KA}).

C arm: A fixed or mobile Xray system used for diagnostic imaging and for fluoroscopic guidance during minimally invasive procedures. The name C arm is derived from the C shaped arm that connects and maintains fixed in space, the Xray source and Xray detector.

Collimation: The process of shaping the Xray beam to minimise the radiation field size to the required area of interest using metallic apertures within the Xray source.

Computed Tomography Angiography (CTA): The combination of Computed Tomography cross sectional imaging with intravenous contrast in order to visualise arterial anatomy and pathology.

Cone Beam Computed Tomography (CBCT): A modality, available in modern endovascular operating rooms, that allows rotational acquisition and provides cross sectional imaging of the patient whilst still on the operating table.

Deterministic effects: Deterministic effects of radiation exposure are related to a threshold dose of radiation exposure above which the severity of injury increases with increasing dose. Deterministic effects include harmful tissue reactions and organ dysfunction that result from radiation induced cell death, e.g. skin lesions and lens opacities.

Diagnostic Reference Levels (DRLs): Used for medical imaging with ionising radiation to indicate whether, in routine conditions, the patient radiation dose for a specified procedure is unusually high or low for that procedure. DRL values are usually defined as the third quartile of the distribution of the median values of the appropriate DRL quantity observed at each healthcare facility.

Digital Subtraction Angiography (DSA): The acquisition of multiple images in succession within one field of view, with the subsequent digital subtraction of images taken prior to contrast injection, leaving a contrast enhanced image of the vessels, and removing non-vascular structures such as bone.

Effective dose: The tissue weighted sum of the equivalent doses in all specified tissues and organs of the body, calculated in Sievert (Sv).

Endovascular operator: Any person carrying out an Xray guided procedure on the vasculature.

Endovascular operating room: Any environment where endovascular procedures are carried out with Xray guidance using a C arm as part of a mobile or fixed imaging system.

Endovascular procedure: Any procedure on the vasculature that uses Xray guidance.

Entrance skin dose (ESD): The dose absorbed by the skin at the entrance point of the Xray beam measured in Gy. This includes the back scattered radiation from the patient.

Equivalent dose: Equivalent dose is the mean absorbed dose in a tissue or organ multiplied by the radiation weighting factor. This weighting factor is 1 for Xrays. Equivalent dose is measured in Sievert (Sv).

European Basic Safety Standards (EBSS) Directive: Describes the standards for protection against the risks associated with exposure to ionising radiation, including radioactive material and natural radiation sources, and also preparedness for the management of emergency exposure situations in the European Union. This is a European Council directive.

Filtration: The materials of the Xray tube window and any permanent or variable or adjustable filters that predominantly attenuate the low energetic Xrays in the beam.

Fluoroscopy time: The cumulative time spent using fluoroscopy during an endovascular procedure.

Gray (Gy): The unit of absorbed radiation dose used to evaluate the amount of energy transferred to matter. One Gy is equivalent to 1 Joule/kg.

Image intensifier: This component of an imaging system relies on the fact that when Xrays are absorbed in a phosphor screen they convert into light photons. These photons impinge upon a photocathode that emits electrons in proportion to the number of incident Xrays. These photoelectrons are then accelerated across a vacuum in an image intensifier to produce an amplified light image.

International Commission on Radiation Protection (ICRP): An independent, international organisation that advances for the public benefit the science of radiological protection, in particular by providing recommendations and guidance on all aspects of protection against ionising radiation.

Medical Physics Expert (MPE): An individual or, if provided for in national legislation, a group of individuals, having the knowledge, training and experience to act or give advice on matters relating to radiation physics applied to medical exposure, whose competence in this respect is recognised by the competent authority.

245

246 **Peak Skin Dose (PSD):** The dose delivered, by both the primary beam and scatter radiation, at the
247 most irradiated area of the skin.

248

249 **Pulse rate:** The number of radiation pulses per second.

250

251 **Radiation exposed worker:** Those over the age of 18 years who may be at risk of receiving radiation
252 doses greater than the stipulated public exposure limit of 1 mSv per year of effective dose.

253

254 **Sievert (Sv):** The unit used to measure both «effective dose» and «equivalent dose». For Xrays,1
255 Sievert equals 1 Gray (Gy).

256

257 **Stochastic effects:** Stochastic effects of radiation exposure are those which occur by chance and as
258 such the probability of them occurring, but not the severity, increases with increasing dose. A Linear
259 No Threshold model has been adopted internationally, acknowledging that there is no threshold
260 dose. The development of malignancy is the most common stochastic effect of radiation exposure.

261

262

263 LIST OF ABBREVIATIONS

264

265	2D	2 Dimensional
266	3D-IF	3 Dimensional Image Fusion
267	AI	Artificial Intelligence
268	AIF	Artificial Intelligence Fluoroscopy
269	ALARA	As Low As Reasonably Achievable
270	AK	Air Kerma
271	ABC	Automatic Brightness Control
272	AEC	Automatic Exposure Control
273	AP	Anterior Posterior
274	APD	Active Personal Dosimeter
275	CAK	Cumulative Air Kerma
276	CBCT	Cone Beam Computed Tomography
277	CT	Computed Tomography
278	CTA	Computed Tomography Angiography
279	DAP	Dose Area Product
280	DICOM	Digital Imaging and Communications in Medicine
281	DNA	Deoxyribonucleic Acid
282	DQE	Detective Quantum Efficiency
283	DRL	Diagnostic Reference Level
284	DSA	Digital Subtraction Angiography
285	E	Effective Dose
286	EBSS	European Basic Safety Standards Directive
287	EJVES	European Journal of Vascular and Endovascular Surgery
288	EM	Electromagnetic
289	ENS	Endovascular Navigation System
290	ESC	European Society of Cardiology
291	ESD	Entrance Skin Dose
292	ESVS	European Society for Vascular Surgery
293	EU	European Union

294	EVST	European Vascular Surgeons in Training
295	eV	Electron Volt
296	EVAR	Endovascular Aortic Repair
297	FDA	US Food and Drug Administration
298	FEVAR	Fenestrated Endovascular Aortic Repair
299	FOV	Field Of View
300	FPD	Flat Panel Detector
301	FORS	Fiber Optic RealShape
302	FT	Fluoroscopy Time
303	GC	Guideline Committee
304	GWC	Guideline Writing Committee
305	Gy	Gray
306	Hp	“personal dose equivalent” in soft tissue below body surface
307	IAEA	International Atomic Energy Agency
308	ICRP	International Commission on Radiological Protection
309	IFU	Instructions For Use
310	II	Image Intensifier
311	IPE	In room Protective Equipment
312	IRR	Ionising Radiation Regulations
313	KAP	Air Kerma Area Product
314	kV	Kilo Voltage
315	kVp	Peak Kilo Voltage
316	LAO	Left Anterior Oblique
317	LAR	Lifetime Attributable Risk
318	LEAD	Lower Extremity Peripheral Arterial Disease
319	LFA	Lead Free Apron
320	LNT	Linear No Threshold
321	mA	Milliamperage
322	MPE	Medical Physics Expert
323	MPR	Multiplanar Reconstructions
324	NCRP	National Council on Radiation Protection and Measurements
325	OCI	Operator Controlled imaging

326	OSL	Optical stimulated luminescence
327	OSLD	Optically Stimulated Luminescence Dosimeters
328	Pb	Lead
329	PPE	Personal Protective Equipment
330	PROSPECT	PROficiency based StePwise Endovascular Curricular Training program
331	PSD	Peak Skin Dose
332	QA	Quality Assurance
333	RAK	Reference Air Kerma
334	RCT	Randomised Controlled Trial
335	RIC	Radiation Induced Cataract
336	RNA	RiboNucleic Acid
337	ROI	Region Of Interest
338	Sv	Sievert
339	TAAA	Thoraco-abdominal Aortic Aneurysm
340	TEVAR	Thoracic Endovascular Aortic Repair
341	TLD	Thermoluminescent Dosimeter
342	UK	United Kingdom
343	UNSCEAR	United Nations Scientific Committee on the Effects of Atomic Radiation
344	VR	Virtual Reality
345		

Chapter 1. Introduction and general aspects

1.1 The need for radiation protection guidelines

The past two decades have witnessed an exponential rise in the number of Xray guided minimally invasive procedures in vascular surgery.¹⁻⁴ With time, many of these endovascular procedures have been validated and have established themselves as the preferred treatment modality based on lower morbidity, mortality, and reduced length of hospital stay, compared with the open surgical alternatives. A large proportion of all vascular interventions are now performed using Xray guided endovascular techniques. Advances in technical expertise, evolving materials technology and improved imaging capabilities have led to increasingly complex endovascular solutions which are associated with prolonged fluoroscopy times and consequently a rise in radiation exposure to both the patient and the endovascular operating team. There is growing concern regarding the increasing radiation exposure, to the patient, and to the whole endovascular team.^{5,6} Endovascular operators are key personnel for promoting radiation safety and should work with other key stakeholders in a team approach to protect the patient and all healthcare staff in the endovascular operating room. The risks of radiation exposure are not universally recognised by all, however, because of a poor understanding of key concepts and paucity of educational material directly relevant to vascular surgery.⁷ The present guidelines on the subject of radiation safety are the first to be written under the auspices of a vascular surgical society. Their explicit aim is to inform the reader about radiation physics and radiation dosimetry, raising awareness of the risks of ionising radiation, and describing the methods available to protect against radiation exposure. Key issues of relevance to radiation protection for endovascular operators and all allied personnel have been outlined, and recommendations provided for best practice. This will no doubt also result in better radiation protection for the patient but a focus on patient radiation protection has been reserved, including during diagnostic procedures that require radiation exposure, for future iterations of the guideline.

The guideline was written and approved by 14 members who, as well as vascular surgeons and interventional radiologists, included a Radiation Protection Scientist and a Medical Physicist. The collated work is based on the best available evidence but also relies on the expert opinion of the aforementioned individuals who, as part of the process of gathering the evidence, identified several areas where future studies would better guide opinion. The reader should note that this document offers guidance and does not aim to dictate standards of care.

1.2 Methodology

1.2.1. Strategy

The grading of each recommendation in these guidelines was agreed by a virtual meeting on 18th February 2022. If there was no unanimous agreement, discussions were held to decide how to reach a consensus. If this failed, then the wording, grade, and level of evidence was secured via a majority vote of the Guidelines Writing Committee (GWC) members. The final version of the guideline was submitted in July 2022. These guidelines will be updated according to future evidence and to the decisions made by the European Society for Vascular Surgery (ESVS) Guidelines Committee (GC).

1.2.2. Literature search and selection

The GWC performed a literature search in Medline (through PubMed), Embase, Clinical Trial databases, and the Cochrane Library up to July 2022. Reference checking and hand search by the GWC added other relevant literature. The GWC selected literature based on the following criteria: (1) Language: English; (2) Level of evidence (table 1). (3) Sample size: Larger studies were given more weight than smaller studies. (4) Relevant articles published after the search date or in another language were included, but only if they were of paramount importance to this guideline.

1.2.3. Weighing the evidence

The recommendations in the guidelines in this document are based on the European Society of Cardiology (ESC) grading system. For each recommendation, the letter A, B, or C marks the level of current evidence (Table 1). Weighing the level of evidence and expert opinion, every recommendation is subsequently marked as either Class I, IIa, IIb, or III (Table 2).

It is important to note that for the general aspects of radiation safety, international bodies such as the International Commission on Radiological Protection (ICRP), the American Association of Physicists in Medicine, the European Federation of Organisations for Medicine and the International Atomic Energy Agency (IAEA) regularly carry out a thorough synthesis of available evidence to publish guidance documents and inform legislation pertaining to safety standards. Legislation in this context refers to statutory regulations that form the main legal requirements for the use and control of ionising radiation. These overview documents, rather than individual literature citations, have been used in the present guidelines to inform recommendations where this was thought to be appropriate. The present radiation protection guidelines are unique in that several of the recommendations made are actually based on legislation that derives from physics principles and extensive, irrefutable evidence that is the basis of this legislation. There have been extensive discussions within the GWC and Guidelines Committee as we have not been confronted previously with this issue in other guidelines. The conclusion agreed between all parties involved is that we could not make recommendations for what are legal requirements but that it is important for the guidelines to highlight areas where law “must” be followed. For this reason, we have, by unanimous decision, used the wording that recommendations based on legislation “must” be followed and the level of evidence has been marked as “law”. It must be noted that in some instances these are not “global or universal laws” and that the level of evidence denoted as “law” means law under most jurisdictions. The recommendations that are based on law are automatically Class I or III. This guideline also has several recommendations, where the evidence is based on physics principles and

the results of studies are absolute truths even in small series. For example, increasing distance from the source of radiation reduces the amount of exposure. This is a principle of physics. The level of evidence used to make this type of recommendations reflects this concept and each of these recommendations is marked with a footnote as a “physics principle.”

Table 1. Levels of evidence according to European Society of Cardiology.

Level of evidence A	Data derived from multiple randomised clinical trials or meta-analyses.
Level of evidence B	Data derived from a single randomized clinical trial or large non-randomised studies.
Level of evidence C	Consensus of opinion of the experts and/or small studies, retrospective studies, registries.

Table 2. Classes of recommendations according to European Society of Cardiology.

Classes of recommendations	Definition
Class I	Evidence and/or general agreement that a given treatment or procedure is beneficial, useful, effective.
Class II	Conflicting evidence and/ or a divergence of opinion about the usefulness/efficacy of the given treatment or procedure.
<i>Class IIa</i>	<i>Weight of evidence/opinion is in favour of usefulness/efficacy.</i>
<i>Class IIb</i>	<i>Usefulness/efficacy is less well established by evidence/opinion.</i>
Class III	Evidence or general agreement that the given treatment or procedure is not useful/ effective, and in some cases may be harmful.

1.2.4. Contributors to guideline.

The GWC was selected by the ESVS to represent both physicians and scientists with expertise in the management of radiation exposure. The members of the GWC have provided disclosure statements of all relationships that might be perceived as real or potential sources of conflict of interest.

The ESVS Guidelines Committee (GC) was responsible for the review and ultimate endorsement of these guidelines. All experts involved in the GWC have approved the final document. The guideline document underwent the formal external expert review process and was reviewed and approved by the ESVS GC. This document has been reviewed in three rounds by 25 reviewers, including vascular surgeons, interventional radiologists and medical physics experts. All reviewers approved the final version of this document.

1.3 The patient and public perspective

1.3.1 Background and aims

Patient and public perceptions of radiation safety pertaining to endovascular surgery were captured. This section was written in partnership with patients and members of the public, to ensure the patient perspective is adequately represented in these guidelines and that medical professionals are aware of these views. The individuals consulted included (i) volunteers from the joint Health Protection Research Unit Public and Community Oversight Committee (<https://crth.hpru.nihr.ac.uk/wider-engagement/>), from the Scottish Environment Protection Agency, and from the Society and College of Radiographers; and (ii) patients who had undergone endovascular procedures at Guy's and St Thomas' NHS Foundation Trust. The group was consulted about the guidelines and asked what they understood by the risks of radiation exposure. The patients' opinion on the information that they would have liked pertaining to radiation exposure prior to their endovascular procedure was sought. We explored whether they would have found this

useful despite the fact that there are many unknowns about the risks associated with low dose radiation exposures.

The following was understood by the group. First that endovascular surgery, involving the blood vessels, referred to as minimally invasive procedures (those which use only small incisions, resulting in the need for only a small number of stitches) is used to diagnose and treat problems affecting the blood vessels (vascular disease). Second that endovascular surgery requires use of ionising radiation, which is radiation of high enough energy to cause damage to cells, potentially resulting in health effects such as cancer. Diagnosis prior to surgery and surveillance commonly requires computed tomography angiography (CTA) using Xrays. It was explained that the use of ionising radiation is in most countries very tightly controlled through legislation, however, the regulations do not cover all the detailed technical aspects of the use of radiation. As such it is important that appropriate guidance is provided to ensure that use of radiation for each specific discipline is justified and safe. We explained that these ESVS guidelines have been prepared by physicians and scientists who are members of the GWC, selected by ESVS on the basis of their expertise in relevant areas of vascular surgery and radiation protection.

The aims of the Guidelines are to outline for medical professionals the key issues of relevance to protect against exposure to ionising radiation. The Guidelines are written for doctors who perform vascular procedures and all allied personnel to provide recommendations for best practice. The Guidelines cover a range of topics including how to measure radiation exposure, the evidence for radiation effects, the current legislation and how to control exposure of the medical personnel through appropriate use of the equipment in the operating room and personal protection, education and training, and the requirements for the future. The Guidelines and recommendations are based on the state of the art in terms of scientific evidence (based on the available studies), as reviewed by the committee, and regular updates are anticipated.

1.3.2 Feedback from stakeholders

The group stated that medical practitioners must have a good understanding of patient perceptions and expectations. In recent years information has become easy to come by, however, the benefits and risks of health effects associated with ionising radiation are not well understood by the non-specialist, and there is a lot of misinformation around. The majority perceived the main risk of radiation exposure to be development of cancer. Further, the real and perceived risk varies greatly depending on the source of radiation and how it is used, as well as on the basis of individual experience. It is generally accepted by the public that imaging involving radiation is an important tool, however, practitioners must ensure that the basic concepts such as what radiation is and why it is being used, as well as the value and risks of the specific procedure are clearly explained to every patient. This can be done both face to face, as part of the consent process, and by providing written literature.

Anecdotally, some patients reported that this has not happened. Some patients also do not feel it is appropriate to question their doctor and they may say that they understand information provided when this may not be the case. The group, therefore, stated that generic literature about the procedures should include specific mention of the radiation risks and that the medical practitioner spends time explaining possible risks to the patient to ensure mutual understanding is reached as far as is practical. The explanation should include a clear explanation to the patient who should be aware that it is acceptable to ask questions. It should also be noted that paediatric exposures are not considered here as endovascular procedures on children are very rare, however, this is something that should perhaps be further considered in future iterations of these Guidelines.

The group stated that it was important for physicians to be aware that the use of ionising radiation in general is based on three principles. First, the principle of justification which requires that use of radiation should do more good than harm. Second, the principle of optimisation requires that

Recommendation 1	Class	Level	References
Information regarding the risks of radiation exposure must be provided in plain, easy to understand language to patients before undertaking endovascular procedures.	I	Law	EBSS (2013) ⁸

radiation doses should be kept as low as reasonably achievable. Thirdly, the principle of dose limitation requires that the dose to individuals from planned exposure situations, other than medical exposure of patients, should not exceed the appropriate limits. In contrast to non-medical uses of ionising radiation, which are solely process based, medical uses of radiation also depend on the requirements of the individual patient. When ionising radiation is used for medical purposes, exposure of the patient is carried out on the basis of the principles of justification and optimisation. Dose limitation is not considered relevant because a dose of ionising radiation that is too low is undesirable as the images produced may not be of high enough quality to perform a procedure.

1.3.3 Responsibilities of the endovascular operator to justify and explain radiation exposure to patients

Justification of radiation exposure for each procedure ensures that the benefit the patient receives from exposure outweighs the radiation detriment and that associated risks are minimised.

Justification is the legal responsibility of the registered healthcare professional (which may or may not be the vascular surgeon). The medical practitioner then takes responsibility to ensure that the patient understands the potential risks and that they understand and agree that the risks are worth taking, after weighing against the benefit of the procedure. If the procedure is justified, optimisation

ensures that the procedure is carried out in the best possible way to deliver the best medical goal with the least radiation detriment.

In medical settings such as during vascular surgery, where the operator of the imaging equipment is not a radiographer or radiologist, the primary responsibility for ensuring the radiation safety of the patient lies with the medical practitioner. In endovascular surgery, ionising radiation is used only for real time imaging purposes, to allow the surgeon to 'see' what they are doing inside the body. As such, in practice, the vascular surgeons themselves have direct responsibility for how much radiation the patient receives as it is the vascular surgeon who directly controls when and how often imaging occurs (through use of a pedal or similar).

The doses received by patients undergoing endovascular surgery vary depending on a number of factors including the type and complexity of the procedure. There are only a small number of studies which look explicitly at the doses patients receive, and more work is clearly needed here. In general, as discussed in Chapter 2 and Appendix 2, information about the risks associated with ionising radiation exposure come from information gathered through many years of use of ionising radiation in medical and nuclear settings, as well as from experience following atomic bomb testing and radiation accidents. For the doses experienced by patients, direct "tissue reactions" such as skin burns are rare. However, such effects do occur, and the risks and severity vary on a patient by patient basis. Further research is ongoing to better understand and guard against such effects. The patients and members of the public who have contributed to this chapter suggest that future research focuses more clearly on the patient specific dose levels involved in different procedures and how these vary on a case by case basis, which will facilitate clearer discussions on risk between patients and medical professionals prior to procedures being carried out; how cumulative doses might be recorded and used within the medical profession as a whole (something which is not generally done yet), and on the doses received by the practitioners themselves to underpin appropriate protection.

Radiation exposure of the patient who receives specific limited exposure as part of treatment or diagnosis does slightly increase the average risk of late effects such as radiation induced cancer, which depends on cumulative lifetime dose, perhaps up to about 5% for a vascular surgery patient, depending on the type of procedure. However, the combined data from all studies suggests that the risk of developing cancer associated with ionising radiation is very small compared with the overall lifetime risk of all cancers, which is now about 50%. Such a risk is acceptable because it is significantly outweighed by the high risk of early death associated with not having the vascular procedure. Hence the procedure is justified. Patients thought they had very little information about radiation exposure and risks prior to their intervention and universally said they would want more despite the fact that some of the exact risks are unknown. Several felt that being empowered with information, either in the form of written information or a dedicated website, would raise their curiosity and make them want to find out more. They thought it was essential that they were counselled about the risks of radiation exposure prior to their procedure but that it was unlikely that the risks would impact their decision to undergo the procedure.

It was also noted that the current legislation and guidelines (including the present Guidelines) are based on the current state of the art in terms of scientific understanding. With further longer term studies on radiation risk currently underway, things may change in the future. The group confirmed that it is important that these Guidelines are regularly updated to reflect that.

In summary, in recent decades, ionising radiation has become an essential resource to perform more and more complex surgical procedures. In most cases, use of ionising radiation is essential to the success of the procedure and as such, the risks of exposure are clearly outweighed by the need to use radiation to save or extend the life of the patient. These Guidelines were deemed essential to continue to ensure medical processes using radiation are undertaken carefully, responsibly and

appropriately. However, more work, including on the topics outlined above, is needed to better understand patient risks and allow further optimisation in the setting of endovascular surgery.

1.4 Plain language summary

Operations carried out on the blood vessels of the body are increasingly performed by techniques that use stents inserted into the blood vessel under Xray guidance. Inevitably, the Xray used is absorbed not only by the patient but also by operators and there is evidence to suggest that exposure to Xray energy has health consequences. With these guidelines strategies that will help minimise Xray exposure during these operations are outlined. The training and educational needs of colleagues are also discussed to ensure they are well informed about radiation protection measures.

Chapter 2. Measuring radiation exposure and the associated risks of exposure

2.1 Radiation exposure during Xray guided procedures

The European Directive on Basic Safety Standards for protection against the dangers arising from exposure to ionising radiation,⁸ obligates Member States in the European Union to improve radiation safety for patients and workers in medical practice. Occupational exposure during Xray guided procedures is closely related to patient exposure and, therefore, both should be managed using an integrated approach.⁹ Radiation doses for some complex Xray guided procedures are equivalent to several hundred chest radiographs, necessitating quality assurance programmes that include optimal radiation protection. Adequate training in radiation protection includes an awareness of the principles of working with radiation and safe exposure limits and this training should be repeated on a regular basis to ensure that it remains current. The ICRP has recognised that there is a substantial need for education and guidance in view of the increased use of radiation in endovascular procedures.^{10, 11}

2.2 Dosimetric parameters

2.2.1 Direct Dose parameters:

Understanding the metrics and definitions used to evaluate the amount of radiation exposure from various sources is key to raise awareness and promote radiation safety. Gray (Gy) is used to report mean organ doses and Sievert (Sv) to report the equivalent and effective dose. These quantities are not measured directly and are estimated by computational methods. Both quantities may be used for a rough estimation of radiation risks and to compare these risks between imaging procedures.

Table 3. Definitions of direct dose parameters

Gray (Gy) is the unit of “absorbed dose” used to evaluate the amount of energy transferred to matter. **Absorbed dose** is the mean energy imparted to matter of mass by ionising radiation. The SI unit for absorbed dose is joule per kilogram and its special name is gray (Gy).

Sievert (Sv) is the unit used to measure two different quantities:

1. **Equivalent dose:** The mean absorbed dose in a tissue or organ multiplied by the radiation weighting factor. This weighting factor is 1 for X-rays
2. **Effective dose** is the tissue weighted (see section 2.4.1.1) sum of the equivalent doses in all specified tissues and organs of the body

2.2.2 Indirect Dose parameters:

One practical approach to audit radiation exposure during Xray guided interventional procedures is to use the dosimetric information generated by the C arm. The amount of radiation generated is typically expressed as “Air Kerma” (AK), measured in mGy. AK is the quotient of the sum of the kinetic energies of all charged particles liberated by uncharged particles in a given mass of air. The position at which the cumulative air kerma is measured is known as the **patient entrance reference point**, which is located 15 cm from the isocentre in the direction of the focal spot of the Xray tube (Figure 1). This value reasonably represents the air kerma incident on the patient’s skin surface.

Figure 1: Illustration of the patient entrance reference point. Xray source is underneath the table.

Image intensifier (I.I) or Flat Panel Detector (FD) above the patient.

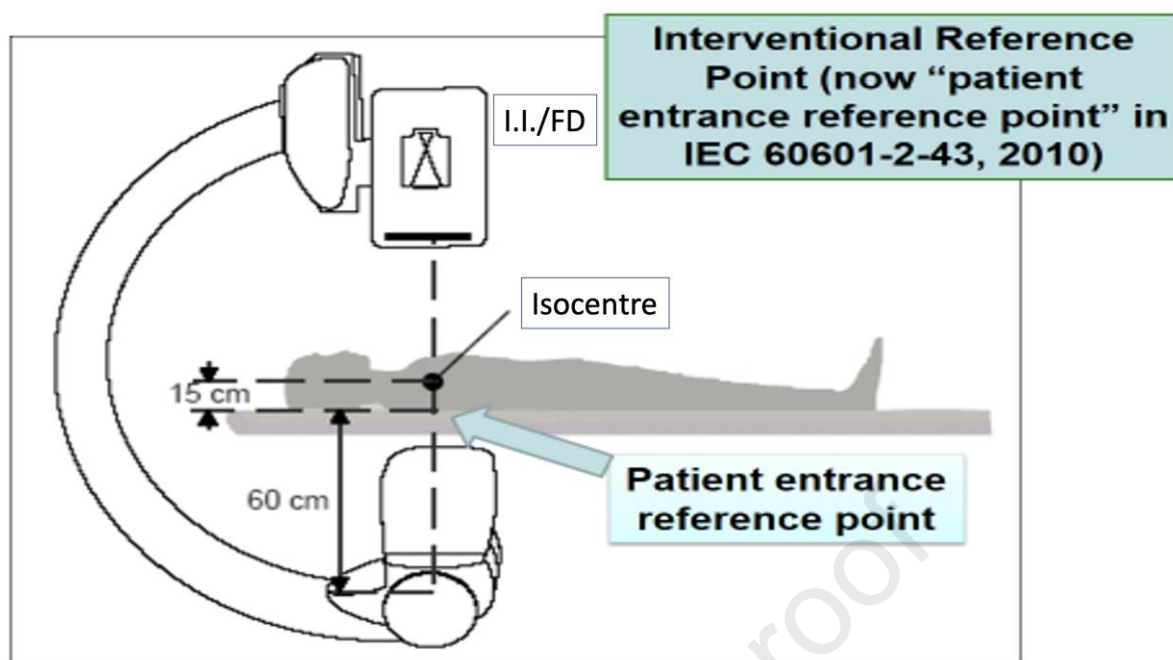


Table 4: Definitions of indirect dose parameters

Air kerma (AK) This is measured in mGy and refers to the dose delivered by the Xray beam to a volume of air and reflects the kinetic energy released in matter.

Air Kerma (AK) at the patient entrance reference point: The AK is measured or calculated at 15 cm from the isocentre in the direction of the focal spot cumulated from a whole Xray procedure (see figure 1), usually expressed in mGy. The selected position reasonably represents the AK incident on the adult patient's skin surface. The US Food and Drug Administration uses the term “**cumulative air kerma (CAK)**” for this parameter.

Air-kerma area product (KAP, or Dose Area product, DAP): The KAP is the product of two factors, namely the air kerma free in air (i.e., in the absence of backscatter) over the area of the Xray beam in a plane perpendicular to the beam axis (usually measured in $\text{Gy}\cdot\text{cm}^2$). The ICRP now recommends referring to those values as Air-kerma area product (P_{KA}).

The C arm can record the rate of delivery of these dose quantities, measured in $\text{Gy.cm}^2/\text{sec}$, during the procedure. Other parameters or related dosimetric quantities, usually included in dose reports produced by the C arm, are the fluoroscopy time (FT) and the number of images (typically digital subtraction angiography (DSA) images) acquired. FT is the cumulative time spent using fluoroscopy and can be used as an indirect dose indicator but its use is limited by the fact that it does not account for the C arm settings, Xray field of view, C arm position or imaging modes used (see chapter 5). Moreover, FT is calculated and displayed differently depending on the C arm and the manufacturer and correlates poorly with other dose indicators.¹²⁻¹⁴ Even though FT can reflect the complexity of a procedure and the efficiency of the operator performing it, dose parameters such as KAP and AK are better for objectively quantifying the amount of radiation exposure and should be used preferentially.¹⁵

2.3 Existing literature informing radiation exposure during endovascular procedures

A literature review was conducted to identify published data on intra-operative radiation doses during endovascular procedures from Dec 2015 – July 2022. The review focused on standard endovascular aortic repair (EVAR), complex EVAR (fenestrated or branched endovascular aortic repair, F/BEVAR) and endovascular treatment of lower extremity peripheral arterial disease (LEPAD), respectively, because these are the most radiating and common procedures in vascular surgery. Deep vein recanalisation procedures were also included, as this is a rapidly developing area of activity on a population that includes young women of childbearing age who may be at particular risk with radiation exposure. The dose parameters collected were KAP (Gy.cm^2), CAK (mGy) and the absorbed doses to which the operators or staff were exposed. The results of this literature review are presented in Table A1 to A3 of the appendix. For the sake of clarity, graphical representations of the available KAP data and a single table are presented in this chapter.

Thirty nine EVAR studies were identified, including 3207 patients with dose reports (based on median KAP) varying by a factor of 28 (from 9.17 (6.83-14.74) to 337 (232–609) Gy.cm^2) (Figure 2, Appendix

Table A1). Reported radiation doses are relatively constant over time with a plateau trend over the period examined. The above lead apron exposure to the endovascular operating team was also reported in several publications and ranged from 5 to 300 μ Sv per procedure.

The highest doses for endovascular procedures were reported for F/BEVAR procedures (Figure 3, Appendix Table A2). Seventeen reports were identified, one was excluded because it reported a mixture of EVAR and F/BEVAR procedures. There is a clear trend toward a reduction in KAP during these complex procedures, which may be a consequence of the learning curve and a wider use of modern imaging equipment. It can also be noted that the published series present increasingly large cohorts. Several studies reported cases in whom intra-operative radiation data exceeded the thresholds (especially $CAK > 5Gy$) that should trigger systemic initiation of dedicated patient monitoring for skin injuries. Not surprisingly, where evaluated, operators' exposures were also higher than during other endovascular procedures (from 120 to 370 μ Sv over the lead apron). Eleven studies, totalling more than 13 000 patients, reported dose parameters during LEPAD endovascular treatment which included crural vessel disease (Figure 4, Appendix table A3). Reported doses tended to be higher for iliac than for femoropopliteal procedures, and for cross over than for anterograde procedures. Radiation data for isolated procedures below the knee were not reported in this analysis. The current data available are limited and heterogeneous. Furthermore, the fact that the leg tissue is thin at this level means that Xrays can readily penetrate and even for long and complex procedures, the radiation dose remains relatively low compared with supra-inguinal procedures.

Only four studies (Table 5) reported radiation dosage during deep vein procedures. It is interesting to note that the dose delivered could reach up to 17.4 mSv, and a little more than one mSv at pelvic level, underlining the need for increased vigilance during these interventions mostly performed in young women.

Figure 2: Graphical representation of studies reporting air Kerma-area product (KAP, Gy.cm²) in the literature between 2015 and 2022 for endovascular aortic aneurysm exclusions (EVAR). The area of each bubble corresponds to the number of patients represented. The dotted line indicates the trend in KAP over time. It can be seen that the published radiation levels are relatively constant with a plateau trend over the period examined.

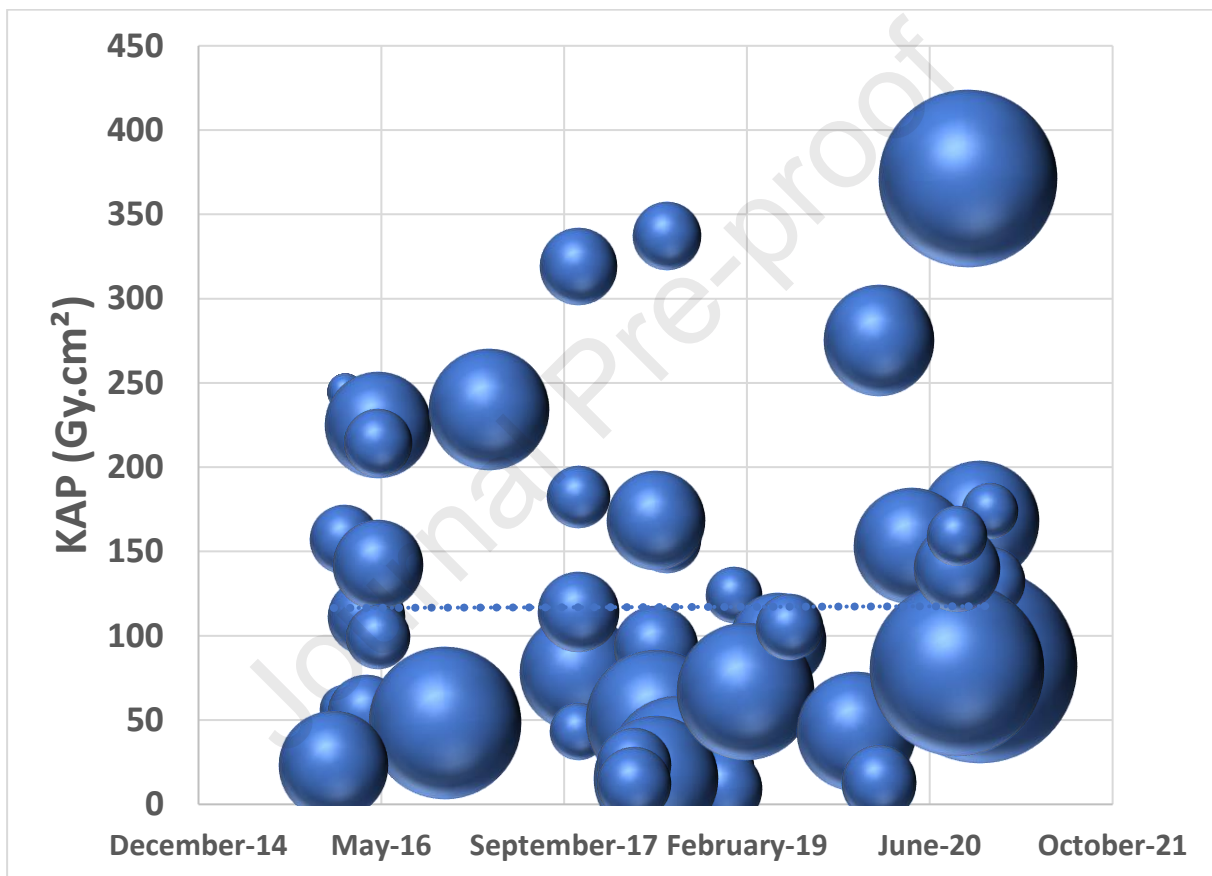


Figure 3: Graphical representation of studies reporting air Kerma-area Product (KAP, Gy.cm²) in the literature between 2015 and 2022 for fenestrated and/or branched endovascular aortic aneurysm repairs (F/BEVAR). The area of each bubble corresponds to the number of patients represented. The dotted line indicates the trend in KAP over time. There is a clear trend toward a reduction in KAP during these complex procedures, which may be a consequence of the learning curve and a wider use of modern imaging equipment. It can also be noted that the published series present increasingly large populations.


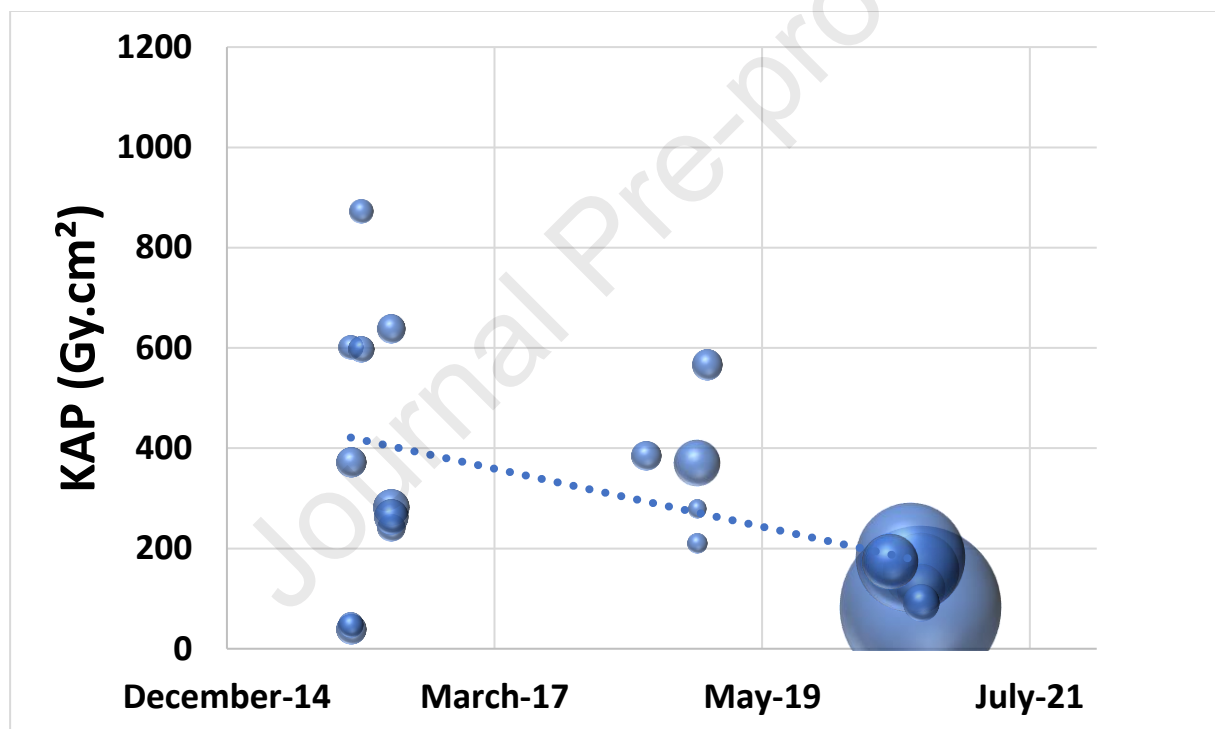


Figure 4: Graphical representation of studies reporting air Kerma-area Product (KAP, Gy.cm²) in the literature between 2015 and 2022 for lower extremity peripheral arterial disease (LEPAD) endovascular treatment. The area of each bubble corresponds to the number of patients represented. The dotted line indicates the trend in KAP over time. There is a clear trend toward a reduction in KAP during these procedures.

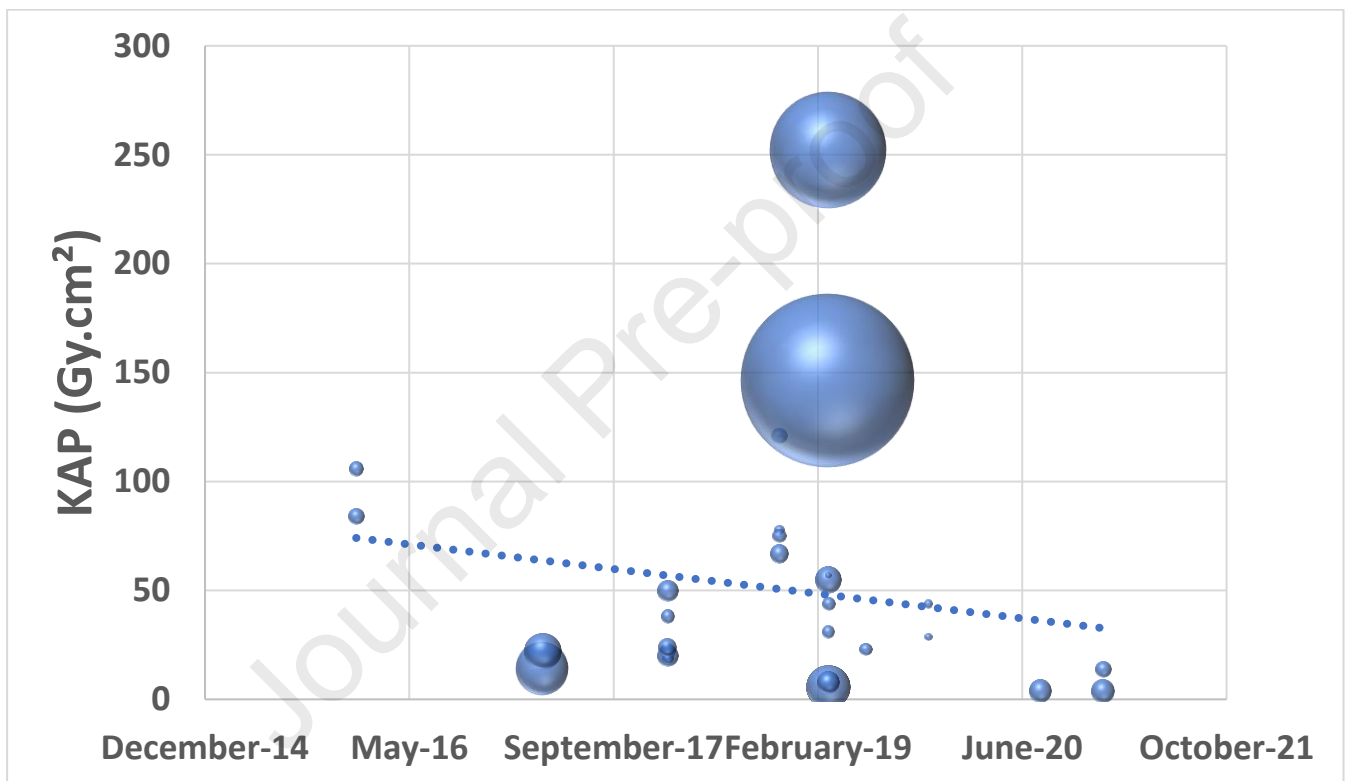

715

716 Table 5: Literature review of published dose reports after endovascular treatment of deep venous
 717 disease between 2016 and 2022. Results are reported in means with standard deviation (SD) or (*) in
 718 median with range, or interquartile range (IQR) if stated. α , Dose measurement above the lead
 719 protections. ALARA: As Low As reasonable Achievable; KAP: Kerma-Area Product; CAK: Cumulative
 720 Air-kerma; DVT: Deep Vein Thrombosis; IVC: Inferior Vena Cava.

721

Author	Year	Groups	Imaging System	Number of procedures	DAP (Gy.cm ²)	CAK (mGy)	Pelvic ESD (mSv)	E (mSv)
Chait ¹⁶	2019	Iliofemoral venous stenting	Mobile C-arm	40	-	1.08 (±0.55)	-	0.221
Barbati ¹⁷	2019	Iliofemoral venous stenting	Mobile C-arm	78	74.6* (IQR 29.5-189.5)	393.5* (IQR 178-955)	1.06* (IQR 9.27-2.59)	17.4* (IQR 7.16-33.12)
Lim ¹⁸	2020	DVT thrombolysis (lower extremity)	Fixed C-arm (endovascular operating room)	20	9.2* (0.2-176.0)	-	-	-

	20	DVT thrombolysis (upper extremity)		91	2.0* (0.1- 11.7)		
		unilateral chronic iliofemoral venous stenting		56	32.4* (0.1- 289.6)		
		-IVC reconstruction		39	60.8* (2.5- 269.1)		
Bacc ellie ri ¹⁹	20	Iliofemoral venous stenting without CBCT	Fixed C-arm (endovascular operating room)	15	24.0* (IQR 19.3– 19.3–35)	69.8* (IQR 19.3– 35)	
	21	Iliofemoral venous stenting with CBCT		10	70.5* (IQR 56.9– 97.3)	244.6* (IQR 190.3– 323.7)	

722

723

724 2.4 Diagnostic reference levels

725 Radiation exposures associated with endovascular procedures can vary significantly

726 depending on the complexity of the procedure (section 2.3). The degree of variability, when

727 the same procedure is performed by different operators and in different centres, suggests that

there should be a move towards standardisation of doses for a particular procedure.^{20,21}

Diagnostic Reference Levels (DRLs) are used in medical imaging with ionising radiation to indicate whether, in routine conditions, the patient dose or administered activity (amount of radioactive material) from a specified procedure, standardised to the patient's height and weight, is unusually high or low for that procedure.²²

The ICRP recommends the use of KAP and AK as the main dosimetric quantities for setting DRLs. DRL values are usually defined as the third quartile (50th – 75th percentile) of the distribution of the median values of the appropriate DRL quantity observed at each healthcare facility.

This allows comparison of local median dose values related to a particular procedure with the recognised DRL for that procedure. Reasons for the doses being substantially higher or lower than the DRL can then be investigated. Fluoroscopy time and the number of acquired images (typically digital subtraction angiogram (DSA) images) may also be used to complement DRLs and to help in the optimisation.

In principle, a DRL could be too low i.e. below which there is insufficient radiation dose to achieve a suitable medical image or diagnostic information. This local review should include the protocols used during the clinical procedures and the equipment setting, in order to determine whether the protection has been adequately optimised. For interventional practices, it is recommended to take into account the complexity of the procedure and its impact on patient dose values. Achieving acceptable image quality or adequate diagnostic information, consistent with the medical imaging task should always be the priority. DRLs should be used to help manage the radiation dose to patients, so that the dose is commensurate with the clinical purpose. A DRL should be used for groups of patients but not be applied to individual patients or considered as a dose limit.^{23, 24} It is acknowledged that there is significant variation in technique, equipment used, as well as the type and severity of disease for each patient, nevertheless, efforts to define outliers in normal practice are valuable with close involvement of medical physics experts to investigate and set DRLs.

Recommendation 2	Class	Level	References
Air-Kerma Area Product (KAP, Gy.cm ²) and the Cumulative Air Kerma (CAK, mGy) must be recorded for all endovascular procedures.	I	Low	NRCP report No. 168 (2010), ¹⁵ ICRP publication 135 (2017) ²³

753

Recommendation 3	Class	Level	References
Establishment of bodies that set national and regional diagnostic reference levels (DRLs) for endovascular procedures is recommended.	I	C	EBSS (2013), ⁸ ICRP publication 135 (2017), ²³ Rial et al. (2020) ²⁴

754

Recommendation 4	Class	Level	References
Review of patient dose values for endovascular procedures at each centre and comparison with the national diagnostic reference levels (DRLs) is recommended.	I	C	EBSS (2013), ⁸ ICRP publication 135 (2017), ²³ Rial et al. (2020) ²⁴ , Farah et al. (2020) ²¹

755

756 2.5 Biological risk related to radiation exposure

757 The following section provides an overview of the biological risks of radiation exposure, with a review
758 of literature related to the biological effects of radiation exposure.

759 2.5.1 Stochastic and Deterministic Effects of Radiation Exposure

760 The harmful effects of ionising radiation can be divided into deterministic and stochastic effects.

761 Stochastic effects are those which occur by chance and as such the probability of them occurring, but

not the severity, increases with increasing dose. There is no threshold dose. The development of malignancy is the most common stochastic effect of radiation exposure. Non-stochastic, deterministic effects, or 'tissue reactions', are related to a threshold dose of radiation exposure above which the severity of injury increases with increasing dose. Deterministic effects include harmful tissue reactions and organ dysfunction that result from radiation induced cell death. Two examples of tissue reactions that occur after radiation exposure are skin lesions and lens opacities.²⁵⁻²⁸

2.5.1.1 Estimators of stochastic risks

The Lifespan study, monitoring the victims of the Hiroshima and Nagasaki nuclear bombs, has shown that the incidence of solid cancers increases proportionately after high and moderate radiation exposures.²⁹ In the medical field, however, both patients and operators are exposed to much lower, although repeated, doses of radiation (< 100 mSv) compared with the high exposures that these bomb victims received in a single, acute manner. Reliable evidence does not exist, therefore, to inform risk associated with exposures below 100 mSv. The Biological Effects of Ionizing Radiation VII (BEIR VII) report and ICRP recommendations, however, conclude that with exposures below 100 mSv, the likelihood of stochastic effects occurring remains proportional to the amount of radiation exposure, and is not threshold dependent i.e. even the lowest exposures could represent a risk to humans.³⁰ This is known as the linear no threshold (LNT) model. While alternative models to LNT have been proposed which may better reflect the radiobiological complexity for certain endpoints, it should be noted that the aim here is provision of a pragmatic tool for estimation of all cancer risk, for radiation protection purposes only.^{31, 32} As such, the scientific consensus remains that LNT remains the model for practical radiation protection.

Stochastic risk is determined by calculating the effective dose (E) of radiation exposure, measured in Sv, where E is the cumulative dose absorbed by organs and tissues, taking into account individual organ/tissue sensitivities to radiation. E represents the same stochastic risk as a uniform equivalent

whole body dose of the same value. The most radiosensitive organs are the bone marrow, colon, lung, stomach and breast.^{28, 33}

The E represents an estimation of stochastic risk in an average individual given a certain amount of radiation. The estimate is not always reliable as it requires complex calculations and mathematical modelling, for example Monte Carlo simulations.³⁴⁻³⁶ Given the different types and amounts of radiation exposure, these stochastic risk estimates are, therefore, not recommended for routine audit purposes and are more useful for estimating theoretical risk in specific cohorts such as pregnant individuals (See section on pregnant exposed 3.3).

Estimation of risk related to radiation exposure should also take into account the age and sex of the individuals exposed. Of note is the fact that endovascular procedures are more frequently carried out in the elderly and less often in paediatric patients. Given that stochastic effects correlate with time after exposure, therefore, elderly patients are at less excess lifetime malignancy risk. For example, the lifetime attributable risk (LAR) of cancer after a coronary computed tomography CT scan in a 80 year old woman would be 0.075% (one induced cancer for 1338 scans), but would rise to 0.7% (one cancer induced for 143 examinations) for a 20 year old woman.³⁰ This issue is further complicated by the use of multiple scans in some patients, particularly younger patients.³⁷

The assessment and interpretation of effective dose from medical exposures of patients also needs to consider that some organs and tissues receive only partial exposures or a very heterogeneous exposure, which is the case especially with diagnostic and interventional procedures.²³

2.5.1.2 Estimators of deterministic risks

Entrance skin dose (ESD, in Gy) is the dose absorbed by the skin at the entrance point of the Xray beam. The Peak Skin Dose (PSD) is the dose delivered, by both the primary beam and scatter radiation, at the most irradiated area of the skin. PSD is used as a predictor for the occurrence of deterministic effects (also called tissue reactions) which are mainly radiation induced dermatitis and erythema and can occur in Xray guided procedures once the radiation exposure to the skin exceeds a given threshold

dose. This risk of skin radiation injuries derived from high dose endovascular procedures are considered in some countries, as an “unintended medical exposure” and necessitate recording, analysis and declaration to the competent authority. The patient is also informed, and arrangements are made for appropriate clinical follow up.

Skin dose can be measured with either thermoluminescent dosimeters (TLDs),³⁸ radiochromic films,³⁹ or optically stimulated luminescence dosimeters (OSLD).⁴⁰ (See Chapter 4). Air Kerma (AK) at a reference point can also be used as a surrogate to assess the risk of deterministic effects, however, it is not always a good indicator for PSD as the Xray beam angulation may be modified during the procedure and the irradiated skin area may be different. Both KAP and CAK can be used to avoid skin injuries when using them as trigger values.⁴¹

Some state of the art fixed C arms incorporate software that displays skin dose maps and peak skin dose during procedures (Figure 5).⁴²⁻⁴⁴ This can prompt proactive intra-operative measures, such as adjusting the C arm angulation, in an effort to avoid persistently irradiating the same skin area during the case. This type of dose measurement and depiction is also valuable to determine whether clinical follow up for potential skin injuries should be considered.^{45, 46} Skin dose map systems should be validated by a medical physics expert (MPE) as the performance of individual systems and their quality varies.

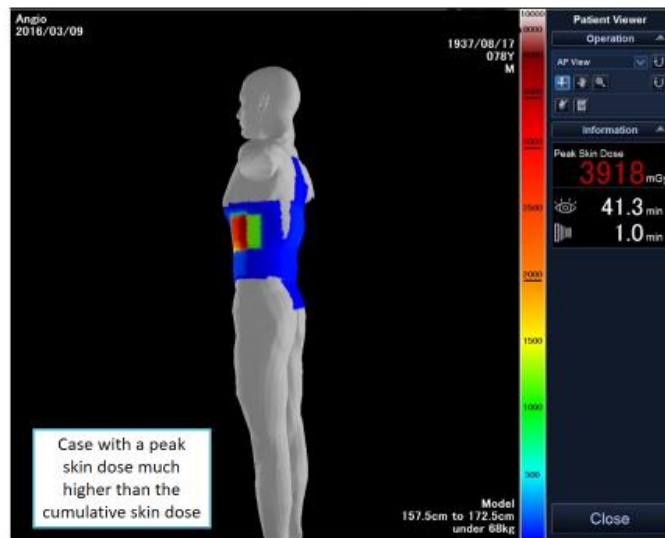


Figure 5: Example of a skin Dose Map software. The area on the left flank depicted in red represents a peak skin dose that is much higher than the cumulative skin dose.

Patient dose values after Xray guided procedures must be registered, allowing protocols to be implemented to decide whether clinical follow up for potential skin radiation injuries is advisable. Suggested thresholds that indicate high risk of skin injuries and should prompt closer patient follow up are:⁴⁷

1. Peak skin dose, more than 3 Gy
2. Air Kerma at the patient entrance reference point: 5 Gy
3. Kerma-area-product: 500 Gy cm²

It is good practice to centrally store patient dose values using dose registration software and regularly evaluate these. This is an important tool for both optimisation of radiation doses as well as for training staff (See section 2.3 and 8.2.8)

2.5.2 The biological response to radiation exposure

Ionising radiation causes damage to cells either directly, by energising nucleic acids in cells, or indirectly, through interaction with the molecular environment. In either case, this results in the generation of reactive oxygen/nitrogen species, damage to the cellular deoxyribonucleic acid (DNA) structure and the activation of DNA repair mechanisms. This biological response can be detected in the blood of patients and operators who are exposed to low dose radiation. Increased levels of phosphorylated histone protein H2AX (γ -H2AX) and phosphorylated ataxia telangiectasia mutated (pATM), two proteins that are markers of DNA damage/repair, are seen in the lymphocytes of patients and operators after endovascular surgery and return to normal by 24 hours, reflecting DNA damage and repair after exposure.⁶ This response to radiation varies between individuals who are exposed to similar doses, a phenomenon that reflects individual variation in sensitivity to radiation induced DNA damage. Radiation protection to the lower extremities mitigates this damage. Raised levels of γ -H2AX, pATM and p53 have also been detected in patients after cross sectional imaging as well as fluoroscopically guided cardiovascular procedures.⁴⁸ The analysis of cellular γ -H2AX foci has been used to predict that a five fold increase in the estimated lifetime attributable cancer mortality following low dose radiation exposure.⁴⁹

2.5.3 Biomarkers of radiation exposure

The level of expression of the DNA damage response proteins γ -H2AX and pATM in circulating lymphocytes may be used as a biomarker of radiation exposure.⁶ Despite initiation of the DNA repair pathway, misrepair can occur and this can lead to chromosomal aberrations such as dicentrics and micronuclei. Micronuclei have been more frequently detected in lymphocytes isolated from hospital workers chronically exposed to low dose occupational radiation.⁵⁰ Higher dicentre frequencies have been detected in interventional cardiologists and radiologists compared with control populations not involved in fluoroscopically guided interventions.⁵¹ Changes in gene expression have also been found in the lymphocytes of patients after CTA,⁵² which has implications for those who undergo regular CT

surveillance following complex EVAR. There is also increasing evidence that microRNAs (RiboNucleic Acid), non-coding RNAs that post-transcriptionally regulate gene expression, are upregulated in interventionalists following exposure to ionising radiation.⁵³ The cellular responses described above can be technically difficult to measure and do not lend themselves to high throughput analysis. Furthermore, there is a lack of standardisation in identification of biomarkers and none have been validated for chronic low dose radiation exposure in endovascular surgery.⁵⁴


2.5.4 Risks associated with occupational radiation exposure to patients

Patients who undergo endovascular procedures are exposed to radiation during the index procedure and also when post-operative surveillance with CT is required. Long term follow up of the EVAR 1 trial suggested a higher incidence of malignancy in patients who had endovascular as opposed to open aortic aneurysm repair⁵⁵ but the study was not designed for this endpoint. A study similarly found a weak signal that patients have an increased risk of post-operative abdominal cancer after EVAR as opposed to open aortic aneurysm surgery but this conclusion is made less reliable because of multiple confounders.⁵⁶ In patients who have had TEVAR, cumulative radiation exposures over two years can exceed 100mSv.⁵⁷ This level of exposure is estimated to account for up to a 2.7% increase in the lifetime risk of leukaemia and solid tumour malignancies.¹¹

Harmful tissue reactions such as skin injuries (Figure 6) generally occur following relatively high radiation exposures and can be seen in patients within hours to days after exposure. At peak skin doses of 2 to 5Gy, the main risk is development of transient erythema, whereas permanent epilation, ulceration and desquamation occur at higher doses. The risk of radiation induced skin injury is higher after more complex procedures that require a longer fluoroscopy time and multiple DSA acquisitions.⁵⁸ Despite the fact that the threshold of 2Gy is exceeded in up to 30% of EVAR procedures,⁵⁹ skin injuries are not commonly reported. This is also the case for more complex EVAR with higher cumulative doses.⁶⁰⁻⁶² This may be in part due to under reporting as skin injury can

appear up to four weeks after exposure by which time the patient has left the hospital and longer term monitoring of the skin for evidence of damage is not widely practiced.

Figure 6: Skin changes that may appear depending on entrance skin dose (ESD) and the expected timeline for changes to develop.

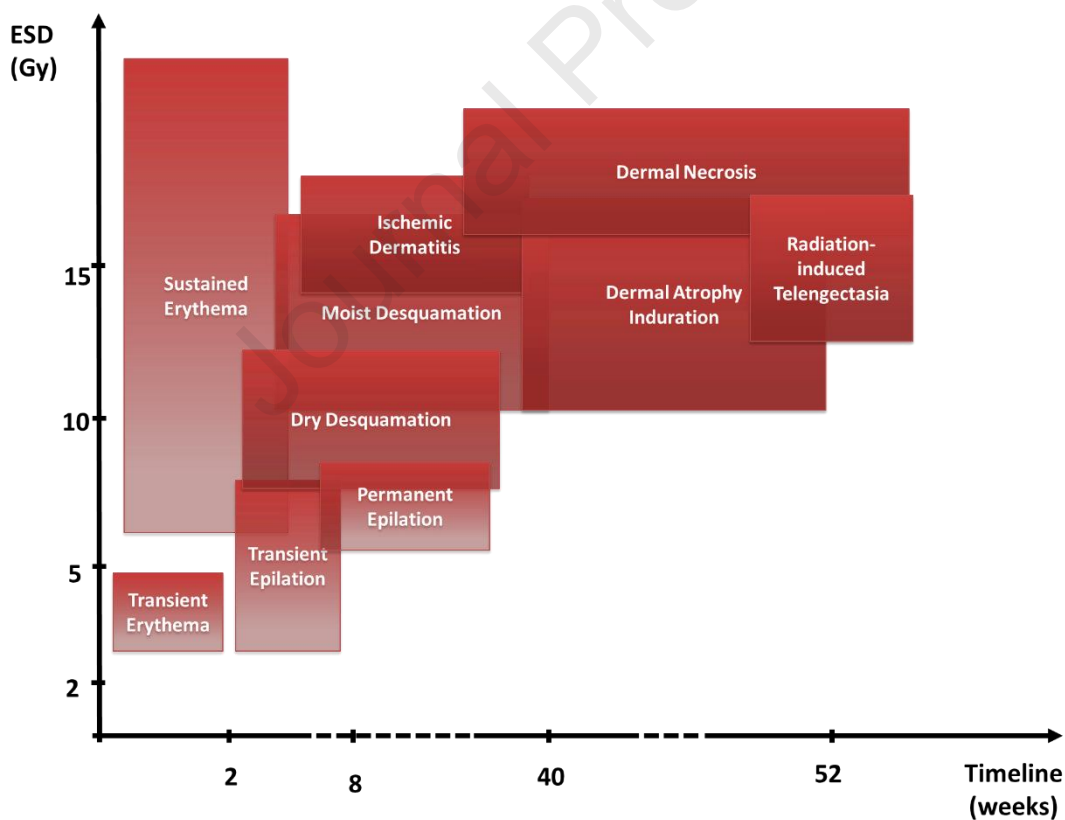

2.5.5 Risks associated with occupational radiation exposure to operators

Reports to date have signalled an increased incidence of thyroid, brain, breast and melanomatous skin cancer after occupational radiation exposure in medical workers.⁶³⁻⁶⁵ Non-melanomatous skin cancers, such as basal cell carcinoma, are also more prevalent after occupational radiation exposure, especially in those with lighter hair colour.⁶⁶ Positive associations between protracted low dose radiation exposure and leukaemia have also been reported.⁶⁷ Overall, medical workers exposed to repeated low dose radiation have a 20% increased risk of cancer when compared with radiation naïve practitioners.^{68, 69} One study found that individuals may have up to a 45% excess cancer related mortality risk after working more than 40 years as an interventional radiologist.⁷⁰ The higher radiation exposure to the left and centre of the head compared with the right⁷¹ and reports of a higher prevalence of left sided tumours in interventionalists suggests the possibility of a causal relationship to occupational radiation exposure⁷². There are, however, other studies that refute a causal relationship between occupational radiation exposure to the head and development of malignant brain tumours⁷³. Multiple confounders, absence of studies in large long term cohorts of workers and an inadequate dose history have meant, however, that there is as yet no conclusive evidence that occupational radiation exposure leads to a higher incidence of malignancy. Better designed longitudinal studies that monitor the long term health effects of radiation exposure in endovascular operators are needed.

Until recently, radiation induced cataracts were thought to be a deterministic sequela of radiation exposures of 5 Gy per single acute exposure and 8 Gy for protracted exposures. It is now thought that lens opacification can occur at exposures lower than 2Gy and that there may, in fact, be no safe dose threshold.⁷⁴⁻⁷⁷ In fact, the increased risk in lens opacity has been reported for doses below 0.5Gy.⁷⁸ It seems that cardiac interventionists have a three to six fold higher risk of cataracts than the general population.^{79, 80}

926 Radiation induced cardiovascular disease is thought to occur as a result of accelerated
927 atherosclerosis; several studies have reported an increase in the risk of cardiovascular disease in
928 patients treated with radiotherapy.⁸¹⁻⁸⁴ Medical radiation workers have, similarly, been found to have
929 a higher risk of ischaemic heart and cerebrovascular disease.⁸⁵

Chapter 3. Legislation regarding exposure limits for radiation exposed workers

3.1 Framework for radiation safety legislation

The legal basis for protection of the public and radiation exposed workers is defined in the European Basic Safety Standards Directive (EBSS).⁸ These standards are developed following detailed review of the published scientific evidence by the United Nations Scientific Committee on the Effects of Atomic Radiation (UNSCEAR) and the ICRP and then agreed through a rigorous process of consultation with relevant bodies, industry, and individual stakeholders within the European Union member states themselves.

The EBSS describes the standards for protection against the risks associated with exposure to ionising radiation. For medically exposed populations, the EBSS particularly emphasises the need for justification of medical exposure, introduces new requirements concerning patient information and strengthens the basis for recording and reporting doses from radiological procedures. It promotes the use of DRLs (see chapter 2) and outlines optimal radiation safety pertaining to endovascular operators.^{8, 86, 87} Justification and optimisation of ionising radiation for medical use are detailed chapter 5.10.

ICRP guidance, published in 2012,²⁸ collated the most up to date research in radiation protection and made a number of recommendations which indicated potential changes to the radiation protection regulations. The EBSS was subsequently updated in 2013 and implemented into European Law in February 2018. The updated EBSS contains a number of changes, most notably highlighting a need for increased protection of the lens of the eye with a revised exposure dose limit. Other notable new stipulations were the recommendations for use of DRLs and the need for recording of dosimetric information by imaging systems and its transfer to the examination report (see chapter 5).


Ultimately, however, the EBSS is a council directive that sets out high level regulations, devolving the responsibility for their interpretation and implementation to the member states.

3.2 Current legislation defining safe radiation exposure limits

Radiation exposed workers are defined as those over the age of 18 who may be at risk of receiving radiation doses greater than the stipulated public exposure limit of 1 mSv per year of effective dose.

It is worth noting that members of the public are exposed to varying levels of natural background radiation, including terrestrial gamma radiation, cosmic rays and radionuclides such as radon. In the United Kingdom (UK) medical radiation exposure accounts for approximately 16% of the 2.7 mSv average annual exposures for members of the public (PHE <https://www.phe-protectionservices.org.uk/radiationandyou/>), the equivalent of approximately 0.43 mSv. The average annual medical imaging effective dose in Europe is approximately 1.1 mSv. In the United States (US), non-therapeutic doses contribute approximately 48% of the average level, but it is worth noting that between 2006 and 2016 the average individual annual medical effective dose from medical radiation has decreased from 2.92 to 2.16 mSv.⁸⁸⁻⁹⁰ Exposures that occur as a consequence of CT imaging account for a large proportion of this medical exposure, significantly increasing in recent years (e.g. figure 7, for the UK). In the same time frame, exposure from conventional Xray has decreased.

Figure 7. UK collective dose from diagnostic Xray procedures.⁹¹

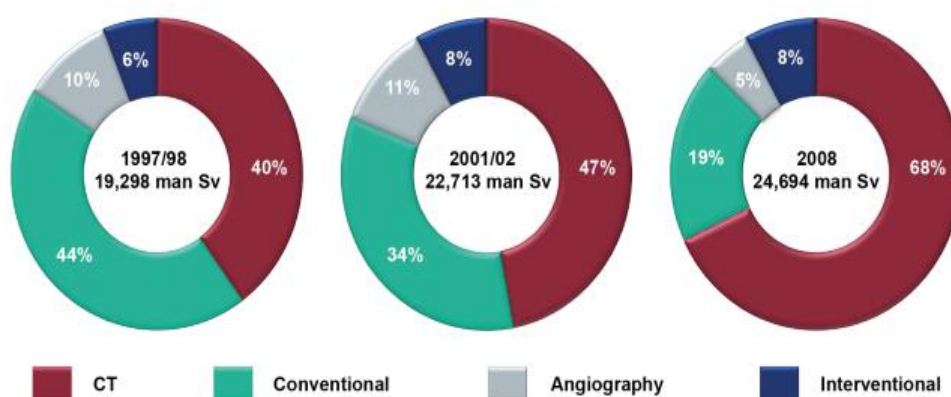

For occupational exposures, including for trainees and students, the effective whole body dose limit is 20 mSv/year. In addition, the equivalent dose limit for the lens of the eye is 20 mSv in a single year or 100 mSv in any five consecutive years subject to a maximum dose of 50 mSv in a single year.⁸ The equivalent dose limit for the skin and extremities is 500 mSv in a year. For the skin this is averaged over any area of 1 cm², regardless of the total area exposed.

Depending on the probable occupational exposure risk, workers may be classified into either category “A” or category “B”.⁸ Category A workers are those likely to (i) exceed an effective exposure dose of 6 mSv/year; or (ii) an equivalent dose greater than 15 mSv per year to the lens of the eye; or (iii) an equivalent dose greater than 150 mSv per year to the skin and extremities. Radiation exposed workers who are not expected to exceed the limits stipulated for category A are classified as category B. Category A workers must be subject to systematic individual monitoring of dose carried out by approved radiation dosimetry service.⁸ A dosimetry service refers to a nationally accredited or otherwise appointed provider of dose monitoring devices, including but not limited to dose badges, as further discussed in Chapter 4. Alternatives to monitoring by a dosimetry service, for category B workers, include estimates based on workplace surveillance or using approved calculations methods. In practice, most member states deal with this by designating category A workers as “classified”. Once designated as classified, they are subject to appropriate evaluation of the magnitude of the likely exposures, optimisation of their radiation protection, education and training and medical surveillance on an annual basis.^{8,9} For category B workers some member states of the European Union (EU) may require individual monitoring but regulations vary from country to country. The advice of a MPE (or radiation protection expert) and a preliminary evaluation of the probable exposure risk is required to categorise the worker into A or B and to decide the individual’s dosimetry and radiation protection strategy. Whatever framework for protection is implemented in practice, there is clear evidence that

1000 interventionists can mitigate the risks associated with ionising radiation exposures by following the
 1001 established safety practices.⁹²

1002 Table 6. Radiation exposure limits set by the European Basic Safety Standards Directive.⁸

1003

Individual	Sub-classification	Annual limits			Additional considerations/Notes
		Whole body	Skin and extremities	Lens of the eye	
Radiation workers	Category A workers (those potentially exposed to > 6 mSv/year effective dose or > 15 mSv/year lens dose)	20 mSv	500 mSv (for skin, averaged over any area of 1 cm ²)	20 mSv (averaged over 5 years but not exceeding 50 mSv in any single year)	Requirement for systematic monitoring based on individual measurements carried out by a dosimetry service, as described in chapter 4.3
	Category B workers (those potentially exposed to < 6 mSv effective dose or < 15 mSv lens dose), including trainees over 18				
	Pregnant workers				The foetus must be protected as a member of the public, i.e. exposure limited to 1 mSv
	Trainees aged 16-18	6 mSv	10 mSv	15 mSv	
Members of the general public		1 mSv			Justification for all medical exposures is a legal requirement. There is no set medical dose limit but exposures should be kept as low as possible

1004

The European Directive on Basic Safety Standards⁸ (Table 6) includes the roles and responsibilities of the “Medical Physics Expert” (MPE). The Directive indicates that the MPE should be involved in interventional radiology practices and should take responsibility for dosimetry, including the evaluation of the dose delivered to the patient. Give advice on medical radiological equipment, contribute to optimisation of radiation protection (including the use of DRLs). The MPE should also contribute to the definition and performance of quality assurance of the medical radiological equipment, the acceptance testing, the surveillance of the medical radiological installations, the analysis of events involving, or potentially involving, accidental or unintended medical exposures and the training of practitioners and other staff in relevant aspects of radiation protection.

Recommendation 5	Class	Level	References
All personnel who may be exposed to ionising radiation in the workplace must comply with European and National legislation	I	Law	ICRP publication 118 (2012), ²⁸ EBSS (2013), ⁸ Casar et al. (2016), ⁸⁷ Stahl et al. (2016), ⁹² ICRP publication 139 (2018), ⁹ Weiss et al. (2020) ⁹³

Recommendation 6	Class	Level	References
Employers must monitor compliance of radiation exposed personnel with legislation regarding radiation exposure limits	I	Law	ICRP publication 118 (2012), ²⁸ EBSS (2013), ⁸ ICRP publication 139 (2018) ⁹

3.3 Pregnancy and radiation exposure

Radiation exposure in the pregnant worker is worthy of special consideration to ensure adequate protection of the foetus. The National Council on Radiation Protection and Measurements (NCRP), Measurements Report on Preconception and Prenatal Radiation Exposure and ICRP document 117 provide comprehensive reviews of the health effects associated with pre-natal doses, as well as guidance on protective equipment (discussed in Chapter 6).^{10, 90, 94, 95} In terms of preconception risks, there is no direct evidence that ionising radiation can cause heritable disease in the children of irradiated individuals.⁹⁶⁻⁹⁸ Pregnant and breastfeeding workers are subject to additional limits with the unborn child subject to the same protection as members of the public. There is evidence that ionising radiation can cause genetic mutations in the foetus that are associated with disease, therefore this risk must be considered and doses to the embryo of > 0.1 Gy may be associated with deterministic risks such as congenital malformations and growth or intellectual disability.^{10, 97} Foetal death is considered a risk only when exposures exceeds 2 Gy, and this is only evidenced by animal studies.^{10, 90, 97} The ICRP 117 report¹⁰ recommends that the foetal dose is kept below 1 mSv during the course of pregnancy for medical radiation workers.⁸ It should be noted that the dose to the healthcare worker and the foetus is usually < 0.3mSv and < 0.1mSV, respectively.⁹⁹ Studies in operators performing endovascular procedures have found minimal exposure to the foetus.^{92, 100} Radiation risks are most significant during pre-implantation and organogenesis and portions of the first trimester, somewhat less in the second trimester, and least in the third trimester.¹⁰¹ More education about the need for special considerations for pregnant workers is needed as this is not well understood by staff and employers.⁹⁵ Perceptions of radiation exposure risk should be managed with a realisation that foetal dose from occupational exposure usually remains well below recommended limits and that female endovascular operators can integrate pregnancy safely into their careers.

A pregnant staff member should be able to seek a confidential consultation with the

the radiation protection expert, MPE, or equivalent to review dose history to determine if any work practice changes are required. More frequent monitoring of radiation dose is usually implemented. The practical difficulties relating to employees' willingness to declare pregnancies prior to 12 weeks gestation, seen as the time after which the pregnancy is most likely to proceed to term, must be acknowledged.¹⁰² The ICRP is clear that discrimination on the basis of gender and potential or actual pregnancy should be avoided, and further specific guidance around ensuring the woman has sufficient radiation protection training and understanding so that she is in a position to make appropriate decisions is also given in ICRP 117.¹⁰ The onus is on the pregnant woman to make the decision regarding when the employer is informed.

A survey of 181 female vascular surgeons found that over half of the 53 respondents became pregnant during training or practice and > 60% performed endovascular procedures whilst pregnant.⁹⁴ With implementation of a programme for declaring pregnancy, assessment of radiation doses and use of adequate protection during pregnancy, it is possible for medical staff to perform procedures and normal activities without incurring significant risks to the foetus.¹⁰³

Recommendation 7	Class	Level	References
A well defined pathway must exist at each institution for pregnant employees to declare their pregnancy in order to manage subsequent occupational radiation exposures	I	Law	Dauer et al. (2015), ¹⁰⁴ Sarkozy et al. (2017), ¹⁰⁵ Shaw et al. (2012), ⁹⁴ Bordoli et al. (2014), ⁹⁵ Stahl et al. (2016), ⁹² Suarez et al. (2007), ¹⁰² ICRP publication 117 (2010), ¹⁰ Chu et al. (2017) ¹⁰³

Chapter 4. Measuring, monitoring and reporting occupational radiation exposure

4.1 Background and Introduction

In contrast to patients who usually have a limited number of higher dose exposures, endovascular operators are regularly exposed to low dose radiation throughout their working lifetime and recording cumulative dose absorbed by the operator is important.^{9, 106-110} The two values that are usually measured by the occupational dosimeters are the “personal dose equivalent” in soft tissue at 0.07 mm below body surface denoted as Hp (0.07) and at 10 mm below body surface, Hp (10). Hp(3mm) is also available for eye lens dosimetry.

4.2. Monitoring radiation exposure during endovascular interventions

Radiation exposure varies depending on the type of endovascular procedure, with more complex procedures carrying a greater radiation burden (see chapter 2).^{111, 112} Radiation exposure is also influenced by the type of C arm used. Mobile configurations and older generation equipment produce images using a higher radiation dose compared with appropriately configured, state of the art fixed imaging systems. Variations in the positioning and operating of the C arm may significantly alter radiation dose to both patients and staff. During endovascular repair of thoraco-abdominal aortic aneurysms (TAAA), a complex Xray guided procedure, the operator effective dose averaged at 0.17 mSv/case.¹¹² One study, measuring radiation exposure during EVAR, found a significant exposure to the temple region of the head (side of the head behind the eyes) of anaesthetists,¹¹³ suggesting that it is important to consider exposures to the entire team and not just endovascular operators. It is recommended that dosimeters are worn by all personnel that are exposed to radiation regularly during work in the endovascular operating room, including trainees, nurses,

circulating nurses, technicians and anaesthetists. Other visiting persons such as medical students and observers may wear a dosimeter if possible.^{9, 33}

The NCRP and the ICRP recommend use of two dosimeters for monitoring radiation exposure, one under lead (shielded by the protective apron, worn on the front of the body, in the area of the main torso, anywhere from waist to neck) and one unshielded above the apron at collar level.^{9, 33, 114, 115} The dosimeter above the apron allows estimating the lens doses, and the combination of the two readings of the dosimeters, provides the best available estimate of effective dose. By recommendation of the NCRP, dosimeter data are used to estimate the whole body exposure (E) combining Hp(10) from both, body/waist (HW) and collar/neck (HN) dosimeters: Effective dose E (estimate) = 0.5HW + 0.025HN.¹¹⁵

The aforementioned use of a dosimeter placed at collar level outside the lead apron provides an estimate of the eye lens exposure but may be supplemented by placing an additional, dedicated dosimeter to measure exposure at the eye level as some endovascular operators may receive annual eye lens doses close to the ICRP dose limit.^{9, 33, 114, 116, 117}

Recommendation 8	Class	Level	References
Two radiation dosimeters, one shielded under the protective apron and one unshielded above the apron, must be worn by all personnel regularly exposed to radiation in the endovascular operating room.	I	Law	ICRP publication 139 (2018), ⁹ ICRP publication 103 (2007) ³³

Additional dosimeters can also be placed on the fingers but an awareness of the risk of sterility issues is advised. Doses for the eyes, hands and feet are generally greater on the side closest to

the radiation source, owing to the position of the operator with respect to the radiation source and direction of travel of the scatter radiation.^{118, 119}

Recommendation 9	Class	Level	References
Endovascular operators may consider wearing additional dosimeters: (i) at the eye level and (ii) on the finger	IIb	C	Bacchim et al. (2016), ¹¹⁴ Albayati et al. (2015), ¹²⁰ Bordy et al. (2011), ¹¹⁶ European Commission Radiation Protection No. 160 (2009) ¹²¹

4.3 Personal radiation exposure monitoring devices

The use of personal radiation monitoring devices and the periodic evaluation of personal dosimetry data promote safer occupational practices.^{122, 123} Regulatory dosimeters are used in radiation safety programs to measure the average monthly occupational radiation dose equivalence to which personnel in the endovascular operating room are exposed. Different personal dosimeters may be used, including passive thermoluminescent dosimeters (TLDs) and active personal dosimeters (APDs). Personal TLD dosimeters are usually processed on a monthly basis and cannot provide real time dose and dose rate information during the procedure. The APDs, however, do provide immediate and continual measurement of radiation exposure that can be visible to the staff member during the procedure. This type of feedback may allow correction of behaviours that result in increased exposure, thereby reducing the cumulative personal radiation dose during the procedure (see chapter 5).^{124, 125}

A thermoluminescent dosimeter (TLD) is a commonly used personal radiation dosimeter consisting of a piece of a thermoluminescent crystalline material inside a radiolucent package.¹⁰⁶ When a thermoluminescent crystal is exposed to ionising radiation, it absorbs and partially traps energy of the radiation in its crystal lattice. When heated, the crystal releases the trapped energy in the form of visible light, the intensity of which is proportional to the intensity of the ionising radiation the crystal was exposed to. A specialised detector measures the intensity of the emitted light, and this measurement is used to calculate the approximate dose of ionising radiation the crystal was exposed to. TLDs have high sensitivity and allow doses lower than 1 mGy and higher than 1 Gy to be accurately measured.¹²⁶

Optically stimulated luminescence (OSL) dosimetry is another well established method of reporting individual doses.¹²⁷ These passive dosimeters work similarly to TLD dosimeters but much faster with a better or at least the same efficiency; but in addition, provide repeated readouts unlike TLD, which is a device that is processed once and is disposable. OSL has also emerged as a practical real time dosimeter for in vivo measurements and may become the first choice for point dose measurements in clinical applications.

Real time dosimeters, also called active personal dosimeters (APD), measure and record radiation exposure in real time and using a wireless connection continuously display the amount of personal exposure.^{128, 129} Besides displaying real time information these systems can optionally emit an acoustic or optical warning when certain real time radiation dose limits are exceeded. The use of this type of dosimetry is increasing and has been shown to reduce radiation exposure to personnel during endovascular procedures.¹²⁹⁻¹³² The accuracy of some APD is questionable, advise from an MPE is thus required when using such devices.

Recommendation 10	Class	Level	References
Real time dosimetry should be considered by all personnel in the endovascular operating room in addition to personal dosimetry.	IIa	C	Müller et al. (2014), ¹³² Chida et al. (2016), ¹²⁸ Inaba et al. (2018) ¹²⁹

1139

1140 4.4 Monitoring and reporting occupational radiation doses

1141 Dose recordings are usually evaluated by an independent service and not by the institution

1142 employing the medical professional. All dose measurements should be performed by an ISO 17025

1143 standard accredited dosimetry service expert in determining equivalent dose estimation to reliably

1144 ensure compliance with dose limits.¹³³

1145 Records of occupational exposure should include information on the nature of the work, exposure

1146 inclusive of all employments, outcomes of health surveillance, education and training on radiological

1147 protection (including refresher courses), results of exposure monitoring, dose assessments and

1148 results of any investigations of abnormal exposure values. Employers must provide staff with access

1149 to records of their own occupational exposure.⁹

1150 Education, training and feedback related to radiation dosimetry should be strengthened. Institutions

1151 must have a dedicated Medical Physics Expert (MPE) and Radiation Protection Officer (RPO) to

1152 manage distribution of dosimeters to staff and monitoring of individual staff exposures.^{134, 135}

1153

1154

1155

1156

Recommendation 11	Class	Level	References
Vascular services should pre-emptively identify personnel who can establish regular pre-determined feedback mechanisms with staff to inform them of personal radiation doses and proactively manage any irregularities to support continuous improvements.	I	C	ICRP publication 139 (2018), ⁹ Sailer et al. (2017), ¹³⁴ Borrego et al. (2020) ¹³⁵

1157

1158 4.5 Inaccuracy and uncertainty associated with personal dosimetry

1159 It must be acknowledged that a failure to wear dosimeters for every procedure, placing the
1160 dosimeter in an inappropriate location on the body and leaving the dosimeter in an environment
1161 where it is exposed to radiation can lead to unreliable cumulative exposure dose values being
1162 recorded. Formulas designed to derive occupational exposures routinely overestimate the actual
1163 effective dose.¹³⁶

Chapter 5. Radiation safety practice in the endovascular operating room

5.1 The “As Low As Reasonably Achievable” (ALARA) principle

The benefits that ionising radiation brings to society, not least to medical science, must be balanced against the stochastic and deterministic risks of health effects (see Chapters 2 and 3). In order to do this, International Commission on Radiation Protection promotes the use of three key principals: justification, optimisation and dose limits. For medical uses of ionising radiation, the justification, that use of radiation must do more good than harm, must always be clear. For patients at least, dose limits are generally not applicable, as the benefits of the use of ionising radiation clearly outweigh the small increased risks and such limits would do more harm than good. For endovascular operators, however, dose limits must be respected.

The key concept in medical radiation protection is thus optimisation, for which is defined the ‘ALARA’ principle: doses to operators and patients must be ‘as low as reasonably achievable’.^{33, 137-142}

In common with all occupational users of ionising radiation, endovascular operators must protect their patients, trainees, the entire team and themselves from the potentially harmful effects of radiation.¹⁴³ Radiation safety begins with developing good habits involving radiation use and protection. Once the basic principles of radiation safety are understood, implementation into daily routines provides a safe working environment for all healthcare providers, personnel and patients involved with the use of radiation. As for all decisions in medicine, the use of Xrays is based on a balance between benefits and risks. The ALARA principle is thus an excellent reference in order to facilitate this.

ALARA protects both the patient and operator. This principle implies that i) a procedure should be performed only if the expected benefits are superior to the potential risks induced by an exposure to Xrays, ii) During the procedure, the lowest radiation doses should be used while maintaining a

sufficient image quality to perform the case safely. The justification for use of ionising radiation should in every case be balanced against the small but non-zero risk of potential adverse health effects, as outlined in Chapter 2, and it is the responsibility of the endovascular operator and indeed every member of staff involved in treatment planning to ensure the appropriate justification applies and that the patient is given appropriate information regarding the radiation risk.

An informed discussion should always be undertaken with the patient, with special care taken to outline the risks and benefits when the procedure involves any of the following:

(i) Paediatric or young patients with anticipated exposure to radiosensitive organs such as eye, breasts, gonads and thyroid gland. Not only are children more sensitive to the effects of radiation than adults but, following radiation exposure, children have a longer post-exposure life expectancy in which to exhibit adverse radiation effects.¹⁴⁴

(ii) Patients weighing either less than 10 kg or greater than 125 kg

(iii) Pregnant individuals

(iv) Procedures anticipated to result in prolonged radiation exposure due to technical difficulty

(v) Repeated exposure to same body region within 60 days

The three components of practice which contribute to ALARA are **time, distance and shielding**.

Minimising the time of radiation exposure is important. Maximising the distance between the body and the radiation source will reduce exposure. Lastly, use of radiation absorbent material, including personal protection equipment, is a key component (Chapter 6.2). The practical aspects of endovascular practice which contribute to ALARA are listed in table 7.

1209 Table 7: Aspects of practice which contribute to the “as low as reasonably achievable” (ALARA)
 1210 principle are a function of three main components: 1. the number of images produced 2. the dose
 1211 required to produce each image and 3. strategies to avoid unnecessary exposure

1212

1. Limit the Number of Produced Images

Use low dose imaging protocols
 Use pulse mode fluoroscopy
 Limit fluoroscopy pulse rate
 Limit fluoroscopy time
 Use advanced imaging techniques (e.g. Image fusion)
 Allow operator control of imaging
 Use DSA algorithms that limit frame rate and the number of images acquired

2. Limit the Dose Required to Produce Images

Use collimation
 Limit C arm angulation
 Optimise detector, generator, and table positions
 Use imaging system auto-exposure settings
 Limit use of digital subtraction angiography (DSA)
 Avoid magnification or use digital magnification
 Use anti-scatter grid removal when appropriate
 Pre-procedural planning

3. Avoid Unnecessary Exposure

1. Use Long Sheaths to maximise operator distance from radiation source
2. Maintain distance from source throughout procedure and exit room during high exposures
3. Use shielding and protective garments

1213

Recommendation 12	Class	Level	References
The As Low As Reasonably Achievable (ALARA) principles must be adhered to by all personnel in the endovascular operating room.	I	Law	ICRP publication 103 (2007), ³³ ICRP publication 105 (2007), ¹³⁷ Hertault et al. (2015), ¹³⁸ Resch et al. (2016), ¹³⁹ Maurel et al. (2017), ¹⁴⁰ Stangenberg et al. (2018), ¹⁴¹ Doyen et al. (2020) ¹⁴²

1214

1215 5.2 Minimising radiation emitted by the C arm

1216 An understanding of basic C arm functions and the operator's interaction with the machine and
 1217 surrounding environment is essential for reducing the dose of radiation emitted. Advances in imaging
 1218 hardware and software have also helped to further reduce exposure. Several imaging modes may be
 1219 used for Xray guided procedures that affect the amount of radiation used, including modes related to
 1220 fluoroscopy, DSA and cone beam computed tomography (CBCT). CBCT refers to a modality, available
 1221 in modern endovascular operating rooms, that allows cross sectional imaging whilst the patient
 1222 remains on the operating table. Similar to standard CT data, the dataset of images can be processed
 1223 on a 3 Dimensional (3D) workstation and represented in multiplanar reconstructions (MPR), 3D
 1224 reconstructions or maximum and minimum intensity projection type reconstruction. The patient
 1225 radiation dose per image (and the image quality) may be very different depending on the settings of
 1226 the Xray system and the pre-defined protocols.

1227 5.3 Low Dose Settings

1228 5.3.1 Fluoroscopy Time and Last Image Hold

1229 One of the most important factors in radiation exposure to both patient and staff is 'pedal time': the
 1230 time the operator has their foot on the pedal that initiates exposure to obtain images.^{145, 146}
 1231 Fluoroscopy should only be used when information is required such as observing objects in motion,¹⁴⁷
 1232 including the use of short taps of 'spot' fluoroscopy when removing wires and catheters and
 1233 inflating/deflating balloons^{145, 147, 148} and disengaging the pedal as soon as data acquisition is
 1234 completed.¹³⁸ Fluoroscopic loop recordings can also be used to review dynamic processes,¹⁴⁷ even
 1235 replacing DSA in some cases. 'Last image hold' is a dose reduction feature available on almost all
 1236 fluoroscopic units to allow interventionists to contemplate images during procedures without the need
 1237 for ongoing exposure and is a mandatory feature by the United States Food and Drug Administration
 1238 (FDA). When Xray exposure is halted the average of the last few frames of fluoroscopy can be displayed

as a 'frozen' image for viewing.^{145, 149-152} It is important to appreciate that different C arms record total fluoroscopy time differently. Some systems record the total number of seconds the pedal is activated (total pedal time), and others use the more accurate accumulation of fluoroscopy pulses (total FT).

5.3.2 Dose Settings & Automatic Brightness Control

The amount of radiation produced by the C arm is dependent on the energy required to generate the Xray beam.¹⁴⁸ This in turn is determined by the milliamperage (mA) and peak kilovolts (kVp) applied across the tube.^{148, 150, 151} The mA and kVp settings control the number of photons produced and image contrast (see appendix 1). The image quality is improved by increasing mA but at the cost of increased radiation.¹⁴⁸

Modern C arms use Automatic Brightness (or Exposure) Control (ABC or AEC) algorithms that optimise image quality by automatically adjusting radiation dose according to feedback from a photodiode within the image intensifier.^{138, 148, 153} If this photodiode detects low image quality, the ABC automatically increases Xray exposure to improve this, increasing the radiation dose without the operator always being aware. It is therefore important to be alert in the following situations where ABC will significantly increase dose: (i) obese patients, (ii) field containing extraneous radiodense material such as body parts outside of the area of interest or metallic objects such as anti-scatter drapes, and (iii) steep gantry angles.

Fluoroscope radiation output is determined by the energy used to generate the beam which is a product of the number of photons produced (mA) and their penetrance (kVp).¹⁴⁸ In addition to the basic mA and kVp settings, modern C arms offer additional low dose settings to reduce radiation dose.¹³⁹ The default settings on most modern machines are usually low dose or extra low dose,¹⁵⁴ but settings can be chosen to further reduce exposure while not necessarily impacting image quality, such as combining an increased kVp with corresponding lower mA.^{112, 148, 150} It may be valuable to seek help

from the manufacturer of C arm equipment to achieve the desired image quality per procedure type at the lowest settings. Increasing the kVp from 75 to 96kVp in this way, with a corresponding reduction in mA, can decrease entrance dose by 50%,¹⁴⁸ with the routine use of half dose settings significantly reducing skin dose with only minor reduction in image quality.¹⁵⁵ This reduction in patient doses is not always involving a similar reduction in the occupational doses for operators.¹⁵⁶ These exposure reductions can be achieved without negatively impacting procedural tasks.^{155, 157, 158} It is important for the responsible person (endovascular operator, radiographer or MPE) to note that dose setting terminology often differs amongst manufacturers.¹⁴⁷

5.3.3 Fluoroscopy and Pulse Rate

Fluoroscopy can be emitted in either a continuous manner, or in short pulsed bursts.^{111, 143, 159}

Continuous fluoroscopy can yield blurred images due to patient and equipment movement whereas pulsed fluoroscopy reduces blurring by counteracting movements, with the additional benefit reducing radiation exposure.¹⁵⁰

Pulsed fluoroscopy is the default mode in modern C arms^{111, 145, 160} with pulse rates typically available at 30, 15, 7.5, 4 and 2 pulses per second. Due to early analogue fluoroscopy initially being developed at 30 frames per second, continuous fluoroscopy was produced at 30 pulses per second. The human eye and the brain's visual reception system can only analyse up to 12 images per second, any more than this are interpreted as an illusion of visual continuity,¹⁶¹ therefore reducing pulse rates from 30 to 15 or 7.5 pulses/second decreases fluoroscopy dose by 47% and 72% respectively^{150, 162} without significantly impacting image quality. The lowest pulse rate that produces an adequate image should be chosen, with studies demonstrating that complex FEVAR can be performed adequately with as low as 3 pulses/second.^{111, 112, 138, 150, 152, 162, 163}

Recommendation 13	Class	Level	References
The use of pulsed rather than continuous fluoroscopy at the lowest pulse rate possible (7.5 pulses per second or less) that produces an adequate diagnostic image is recommended for endovascular procedures.	I	C	Rolls et al. (2016), ¹⁶³ Panuccio et al. (2011), ¹¹² Pitton et al. (2012), ¹⁵² Ketteler et al. (2011), ¹⁵⁰ Hertault et al. (2015), ¹³⁸ Monastiriotis et al. (2015), ¹¹¹ Miller et al. (2002) ¹⁶²

5.3.4 Digital Subtraction Angiography and Frame Rate

Digital Subtraction Angiography (DSA) describes the acquisition of multiple images in succession within one field of view, with the subsequent digital subtracting of non-vascular structures, such as bone, leaving a contrast enhanced image of the vessels. The cost of these multiple high quality images is a substantial increase in radiation dose compared with fluoroscopy,^{138, 164} a fact that seems to be generally underappreciated.¹⁶⁵ The contribution of DSA to total radiation dose during peripheral arterial and cardiac interventions has been shown to range between 70% and 90%,^{152, 166} and accounts for 50 - 80% of the radiation dose during TEVAR and EVAR, even when low frame rates of 2/sec were selected.^{165, 167} DSA frame rate describes the number of images recorded per second, distinct to fluoroscopy pulse rate which describes the number of bursts of radiation the fluoroscope emits per second. Compared with fluoroscopy, DSA is associated with at least 10 fold higher dose rate per frame,¹⁶⁴ contributing to 66% of the radiation dose while only accounting for 23% of total exposure time.¹⁶⁸ The patient entrance dose for one fluoroscopy image may be 10-30 μGy , 100-300 μGy for one fluoroscopy loop and 1000-3000 μGy (or more) for one DSA image. For operators, DSA leads to an eight fold higher radiation dose than fluoroscopy.¹⁵²

If DSA runs are essential, the associated dose can be minimised by (i) reducing the number of pictures acquired per second (frame rate); (ii) minimising time per run; and (iii) limiting the number of acquisitions.¹⁴⁷ Reducing the frame rate will reduce dose in the same way as reducing pulse rate during

fluoroscopy,^{112, 147, 152, 165} with number of frames correlating highly with total radiation dose.¹⁵² Reducing frame rates to 7.5 fps from a continuous mode, for example, results in a 90% reduction in image numbers, with an equivalent reduction in radiation dose.¹³⁸ Adequate images can be obtained even with frame rates of 2 frames per second (fps) for pelvic and upper leg interventions and 1 fps for lower leg and foot interventions.¹⁵² It should be noted that CO₂ angiography often needs higher frame rates (4-6 fps) to obtain adequate images and may be associated with higher radiation doses.^{169, 170} Some systems allow a Variable Frame Rate setting which reduces the frame rate once adequate vessel opacification has occurred and this may help further reduce radiation usage.

One of the most effective techniques for reducing radiation dose during endovascular procedures is to limit DSA acquisitions to key scenes and critical steps during the procedure.¹⁵² If high quality imaging is not essential then fluoroscopy loops can often replace DSA.^{111, 138, 151, 152, 160, 165, 171, 172} The endovascular operator needs to determine the lowest quality image that still maintains safety by allowing effective diagnosis, and treatment at all times during the procedure.¹⁵⁰ Modern C arms reduce the need for repeated DSA by allowing overlay roadmap of a DSA for target cannulation and the ability to return the table to the exact position and overlay a fade of a previous DSA.¹⁵² Some C arms also allow this to be done using fluoroscopy, avoiding the extra radiation required for DSA to perform this function.

Recommendation 14	Class	Level	References*
It is recommended that use of Digital subtraction angiography (DSA) be limited to critical steps during endovascular procedures, and that it is carried out with the shortest time per run, lowest frame rate and least number of acquisitions possible to acquire an adequate image.	I	B	Pitton et al. (2012), ¹⁵² Ketteler et al. (2011), ¹⁵⁰ Hertault et al. (2015), ¹³⁸ Haqqani et al. (2013) ¹⁷¹ *Physics principle


1328

1329 5.4 Collimation

1330 Collimation uses metallic apertures within the Xray source to modify the beam and minimise the
1331 radiation field size to the required area of interest.¹⁷² By shaping the beam and absorbing photons,
1332 collimation not only produces sharper images by hardening the beam, but also reduces radiation
1333 exposure (Figure 8) to the patient and medical personnel in proportion to the reduced image size, with
1334 a consequent reduction in scatter.^{62, 112, 138, 145, 150, 152, 173}

1335

1336 Figure 8: Collimation results in a significant radiation dose reduction from a DAP of 42mGycm² without
1337 collimation (A) to 14Gycm² with collimation (B) for an equivalent screening time.

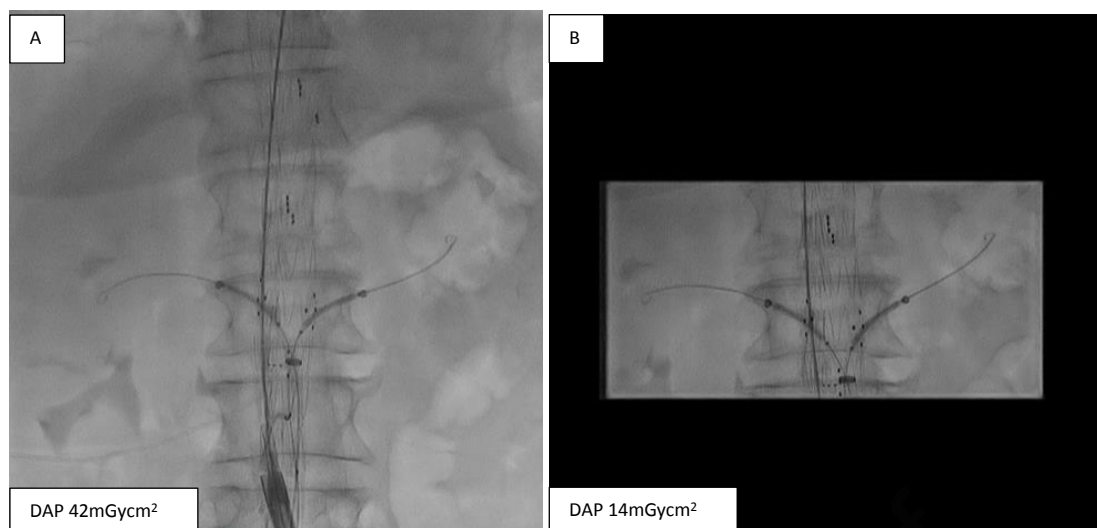

During cardiac procedures, for example, the use of collimation reduces patient and staff radiation by 40%,¹⁷⁴ and meticulously collimating on a modern C arm can reduce KAP by a factor of more than 10.¹⁷⁵ Performing horizontal and vertical collimation significantly reduces scatter independent of each other with a 5cm collimation of each reducing scatter radiation to the operator, assistant and anaesthetist by 86%, 80% and 96% for horizontal collimation and 88%, 89% and 92% for vertical collimation respectively.¹⁷⁶ However, collimation reduces scatter at the cost of increased patient skin entrance dose in some cases.¹⁷⁶ By focusing the radiation field to a smaller area on the patient, a larger volume of the patient's tissues is available to attenuate scatter before exiting the patient and reaching staff.¹⁷⁶ For this reason highly collimated studies should not be performed for prolonged periods of time in one gantry position. Collimation blades can be virtually projected onto the monitor eliminating the need for fluoroscopy to adjust collimation leaf position.^{138, 147} Even when a full field is required the collimator blade edges should be seen just visible on the monitor edges to ensure radiation protection extends outside of the image receptor view.¹⁷²

Recommendation 15	Class	Level	References*
Active use of collimation, even for full field images is recommended for endovascular procedures.	I	B	Ketteler et al. (2011), ¹⁵⁰ Pitton et al. (2012), ¹⁵² Haqqani et al. (2012) ¹⁷⁶ *Physics principle

1355

1356 5.5 Anti-scatter Grid Removal

1357 Detectors are equipped with anti-scatter grids whose role is to filter the Xray beam from scattered
 1358 radiations before it reaches the captor. This decreases the background noise and therefore improves
 1359 image quality. However, those grids are responsible for some attenuation which implies that the
 1360 energy carried by the Xray beam will be higher. In cases where the scatter radiation is minimal i.e.
 1361 when the thickness of tissue to cross is low with minimal scatters, as typically occurs in children,
 1362 arteriovenous fistulae and below knee lesions, removal of the anti-scatter grid can be considered to
 1363 decrease the overall radiation use.¹⁷⁷ Familiarity with imaging equipment and availability of
 1364 personnel to help determine when anti-scatter grid removal is advisable can help reduce overall
 1365 radiation use.

1366

Recommendation 16	Class	Level	References
Anti-scatter grid removal during endovascular procedures should be considered when scatter radiation is minimal.	Ila	C	Gould et al. (2017) ¹⁷⁷

1367

5.6 Dose Reduction Hardware and Software

5.6.1 Advanced Dose Reduction Hardware & Software

The operator must be cognisant of the fact that the excellent quality images achieved with modern C arms can come at the cost of increased radiation dose. This has prompted imaging equipment vendors to focus on methods to reduce radiation dose whilst maintaining imaging quality.¹⁷⁸ All vendors have developed their own proprietary approach combining advances in hardware and software. These dose reduction technologies include (i) machine controls (smaller focal spots, shorter pulses, lower tube current and additional beam filtration), (ii) image processing algorithms (automatic pixel shifting, temporal averaging of consecutive imaging, spatial noise reduction, motion compensation and image enhancement) and (iii) hardware configurations to reduce entrance dose (optimising acquisition chain for different anatomical regions).^{141, 159} Studies comparing upgraded systems to previous iterations have reported halving of radiation use associated with EVAR, 70% reduction in lower extremity interventions, and almost 40% reduction with embolisation.^{141, 159, 179-181}

5.6.2 Pre-Operative Planning Software

Implementation and review of pre-procedural planning software from axial imaging diagnostic studies can be extremely beneficial in enhancing procedural workflow and reduction of ionising radiation use. Performing pre-operative case planning on CT imaging post-processing software on 3D workstations prior to interventions is essential to limit unnecessary diagnostic runs.^{138, 182} Identifying the most appropriate angles for optimal viewing for each step of the procedure, as well as saving appropriate images for reference during the procedure reduces radiation exposure.¹³⁸ Profiling of the iliac bifurcation and the proximal aortic landing zone during EVAR, for example, often requires significant gantry angulation (e.g. 20 - 30 degrees of lateral angulation for iliacs and 5 - 15 degrees cranial angulation for the neck).¹⁸³ Repeated DSA runs carried out in these positions to determine the optimal angle contributes to the highest radiation doses and operator scatter exposure during

EVAR.¹⁸⁴ One study using vendor specific post-processing software resulted in the elimination of unnecessary diagnostic runs with a three fold reduction in mean DAP during EVAR.¹⁸⁴ Other studies using open source software to predict C arm angles pre-operatively have demonstrated a reduction in operating time by one third.^{185, 186}

Recommendation 17	Class	Level	References
Detailed pre-operative procedural planning, including the use of a 3D workstation is recommended to reduce radiation exposure in endovascular procedures.	I	C	Stansfield et al. (2016), ¹⁸² Hertault et al. (2015) ¹³⁸

5.6.3 3D-Image Fusion Software

3D image fusion (3D-IF) describes the combination of pre-operative CTA images with live fluoroscopy, producing a three dimensional volume rendered angiogram which can be used as a virtual roadmap during interventions, particularly useful during complex EVAR.¹⁸⁷ Bony landmarks are co-registered on both the pre-operative and live images and the resultant fused 3D model automatically follows the table and gantry movements.¹³⁸ This negates the need for repeated DSA and fluoroscopy to position the table and gantry for target vessel cannulation and during subsequent stent deployment. This consequently reduces procedure time, contrast use and radiation exposure.^{165, 188, 189} Studies utilising 3D-IF report up to 70% reduction in radiation during standard EVAR and complex aortic repair interventions.^{138, 163, 190-193}

Co-registration of the images at the beginning of the case, however, does add additional radiation with systems requiring a full or partial cone beam CT (CBCT) spin adding approximately 5% of the

total radiation dose of the procedure.¹⁸⁷ Replacing CBCT with two orthogonal anteroposterior (AP) and lateral fluoroscopic acquisitions reduces this additional dose by ten fold.^{163, 194, 195} Another limitation of 3D-IF is inaccuracy of overlay, particularly following vessel deformation caused by the passage of stiff wires and devices, which renders the overlaid pre-op images inaccurate.¹⁹⁶ More sophisticated registration systems have been developed precluding the requirement for a pre-op co-registration Xray,¹⁹⁶ or used cloud based technologies for more accurate overlay with a consequential reduction in radiation exposure, FT and procedural time.¹⁹⁷ Cutting edge advances in 3D-IF use cloud based artificial intelligence (AI) to correct vessel deformation in real time. No randomised controlled trials have been designed to solely study the impact of fusion imaging. A comparative analysis of patients treated with and without fusion in the same environment demonstrated a trend towards lower DAP in the fusion group.¹⁹³ In a meta-analysis of the various studies reporting exposures during after EVAR, fusion was identified as an independent predictor of dose reduction.¹⁹⁸ Guidance with fusion imaging is also being used increasingly for endovascular intervention in LEPAD and evidence for a benefit during these procedures is emerging.¹⁹⁹

Recommendation 18	Class	Level	References
Image fusion should be considered during aortic endovascular procedures to reduce radiation exposure	Ila	B	de Ruiter et al. (2016), ¹⁹⁸ Ahmad et al. (2018) ¹⁹³

5.6.4 Detectors and image intensifiers

5.6.4.1 Image Intensifiers and Flat Panel Detectors

Detectors register Xrays that have passed through the patient from the Xray tube and an image intensifier (II) then converts these photons into light that can be viewed as an Xray image. Traditional

analogue image intensifiers have now been largely replaced with digital flat panel detectors (FPD) which offer better imaging performance. Flat panel detectors have a much higher sensitivity to Xrays, a high signal to noise ratio, wide dynamic range, limited geometric distortion, absence of veiling glare or vignetting, high uniformity across the field of view, advanced image processing, and improved manoeuvrability due to their smaller size.²⁰⁰⁻²⁰²

5.6.4.2 Optimal use of Flat Panel Detectors to minimise Radiation Dose

With improved Detective Quantum Efficiency (DQE) converting Xrays into visible images, FPDs theoretically provide an opportunity to reduce the radiation dose required to obtain images^{202, 203} but this may not be the case in practice. Numerous contradictory studies, using both patients and phantom models have resulted in uncertainty as to whether transitioning from traditional image intensifiers to FPD is associated with a radiation dose saving.^{200, 201, 204} Whilst some reports suggest that patient dose could be reduced by up to 50%,^{203, 205} others have noted that reduced entrance doses do not automatically lead to reduced operator radiation doses in clinical practice, measured by DAP.²⁰⁰ Several studies have reported significantly higher DAP associated with FPDs, up to three times higher, compared with traditional IIs.^{204, 206, 207} Suggested reasons for higher doses are that frame rate settings are typically higher with FDPs than for IIs,²⁰⁸ and the additional sensitivity to noise can lead to vendors increasing dose settings to ensure that images are of sufficient quality to satisfy operators.²⁰³ Another factor complicating direct comparisons are that FPDs are often part of more modern angiographic units that incorporate dose reduction strategies, which means the independent effect of the FDP component on dose is more difficult to ascertain.²⁰⁹

FPDs must be optimally configured, and the detector entrance dose rate in relation to the clinical detection task optimised, in order to minimise radiation dose.²⁰¹ In a direct comparison of 11 FPD systems to 9 II systems, failure to use low dose settings available on the emitter system was thought to negate the superiority of FDPs and resulted in comparable radiation doses between the two systems.²¹⁰ Several authors have stressed the importance of specialist assistance from application

engineers in correctly setting up protocols in order to fully use low dose modes and achieve radiation dose savings when using FPDs.^{201, 211} The configuration, optimisation and calibration of settings include fluoroscopy pulse rate, detector entrance dose, tube voltage, filtration, frame rates and post-processing imaging parameters, and these all need to be balanced against adequate image quality for clinical use.^{200, 201, 210} Due to their increased DQE low dose or extra low dose modes should routinely be chosen over normal modes, as these are associated with a large radiation saving whilst maintaining excellent imaging quality.^{195, 203} Reducing detector entrance dose from one setting to the next lowest setting doesn't dramatically change the image quality, but has the potential to reduce radiation dose by 15%.²⁰⁶

Recommendation 19	Class	Level	References
Flat panel detectors should be considered in preference to image intensifiers in an effort to improve imaging quality and reduce radiation exposure	Ila	C	Livingstone et al. (2015), ¹⁹⁵ Bokou et al. (2008), ²⁰¹ Suzuki et al. (2005) ²⁰⁹

5.7 Magnification

5.7.1 Conventional Magnification

Detectors are available in a range of sizes, referred to as input Field Of View (FOV). Using the largest FOV available results in the lowest output spatial resolution and highest image distortion, but with the lowest radiation dose. This relationship is system specific. Irradiating a smaller area of the detector gives the effect of magnifying the image. If the FOV is halved, the spatial resolution is doubled thereby improving visibility.²¹² The area irradiated is proportional to the square of the FOV, therefore, only a quarter of the input detector is irradiated, reducing the image brightness to a quarter of the original

FOV, making it too dark to view if all other parameters are kept constant.²¹² In this scenario the machine's ABC quadruples the radiation to compensate and deliver a bright usable image (Figure 9).²¹³ In general, the smaller the FOV, the greater the magnification, and the higher the patient dose.²¹² In order to avoid irradiating non-visualised areas during magnification, collimation is applied automatically, or must be set manually. This increases entrance skin dose but reduces scatter to the operating team, therefore, a smaller FOV (increased magnification) increases CAK but decreases DAP.⁷ Endovascular Operators are therefore advised to use the largest FOV as possible with judicious use of magnification.^{146, 148, 151}


5.7.2 Digital Zoom

An alternative method of achieving image magnification whilst avoiding the increased radiation dose associated with conventional magnification is to instead acquire images using digital magnification (also known as digital zoom). When combined with large monitors this can produce a similar effect.^{138, 147} These monitors are typically greater than 1.5m in diagonal dimension. Some C arms offer 'Live Zoom' where the image is digitally enlarged in real time, with up to 2.5 fold saving in radiation dose compared with conventional zoom.²¹⁴ It has been estimated that the use of digital zoom can reduce dose by up to 30% compared with changing FOV.²¹⁵ A recent study demonstrated that use of digital zoom during coronary procedures was not inferior to conventional zoom in a blinded test for visibility, and furthermore was associated with a saving in radiation dose of approximately 30%, with reductions in both RAK and DAP.²¹⁴

Recommendation 20	Class	Level	References
Digital zoom, rather than conventional magnification, and appropriately sized monitors are recommended for the reduction of radiation dose during endovascular procedures	I	C	Hertault et al. (2015), ¹³⁸ Machan et al. (2018) ¹⁴⁷

1498

1499 Figure 9: Impact of magnification on image quality and radiation exposure. Magnification
 1500 results in resolution loss. In order to maintain image quality an increase in dose exposure is
 1501 required.

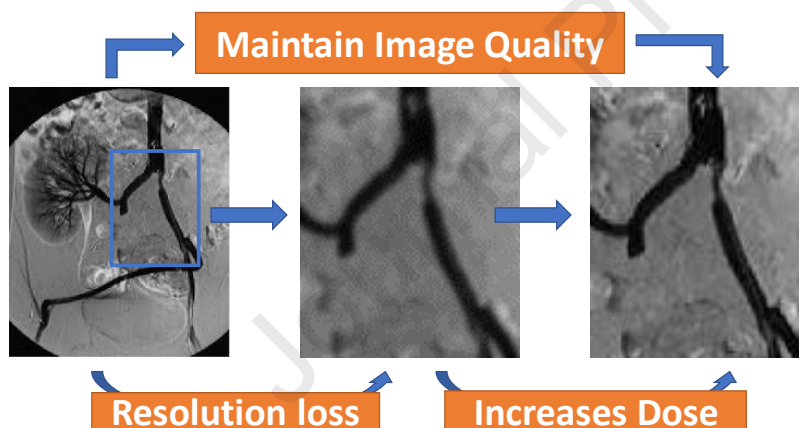

1502

1503 5.8 Dose reports from modern Xray machines

1504 Modern Xray systems are able to give detailed information on the radiation dose associated with
 1505 fluoroscopy, DSA and CBCT. This information is very useful for optimising radiation protection as it
 1506 allows endovascular operators to determine how much radiation exposure occurs during each of the
 1507 three aforementioned manoeuvres in order to alter their behaviour accordingly. In fact, most modern
 1508 Xray systems now report live values of air-kerma area product (KAP) and cumulative air kerma (CAK)
 1509 as well as cumulative values at the end of the case. This circumvents the need to analyse the Digital

Imaging and Communications in Medicine (DICOM) dose structured reports that contains the full details of dose per radiation event and has traditionally been used to obtain these data. All dose monitoring data should be recorded at institutional level.

Recommendation 21	Class	Level	References
Real time dose information must be provided by the C arm to optimise radiation protection during endovascular procedures	I	Law	EBSS (2013) ⁸

5.9 Maintenance

Radiation systems must be included in ongoing quality assurance (QA) programmes to ensure they are maintained in prime working condition, remain efficient and are regularly calibrated, to ensure that high quality images are obtained using the lowest possible doses, and dosimeter readings remain accurate.^{138, 164} A ten point check list designed to improve medical radiation safety culture in the UK includes evidence of appropriate management of radiation equipment and radioactive materials.²¹⁶ This includes documented evidence of management systems, equipment replacement programmes, service and maintenance contracts, QA, action on QA results, and audit of RAM policy and procedures. The responsibilities lie with the imaging facility institution through their medical physicist, and are facilitated by the C arm vendor, although legislation in this area varies between countries.

Recommendation 22	Class	Level	References
Maintenance and assessment of ionising radiation equipment must be performed regularly for quality and safety.	I	Law	Hirshfeld et al. (2018), ¹⁶⁴ Hertault et al. (2015), ¹³⁸ Chapple et al. (2016) ²¹⁶

1528

1529 5.10 Endovascular operating rooms: Hybrid suites & interventional platforms

1530 5.10.1 Mobile C arms

1531 Compared with modern fixed systems, mobile C arms generally produce inferior imaging quality, are
1532 prone to overheating and, importantly, can increase exposure to the operator due to a lack of table
1533 and ceiling mounted shields (**refer chapter 6**).^{141, 198, 217-220} In addition, they are associated with inferior
1534 ergonomics. Mobile C arms generate less radiation during EVAR compared with hybrid suites^{24, 198, 221}
1535 leading to suggestions that for standard EVAR mobile C arms are of sufficient quality to perform the
1536 task, with some studies reporting similar fluoroscopy times and outcomes for EVAR performed with a
1537 mobile C arms compared with fixed systems.^{222, 223} In addition mobile C arms are cheaper and more
1538 compact than fixed systems. The counter argument, however, would question the safety of performing
1539 complex or prolonged procedures with inferior imaging capabilities and increased operator dose,
1540 whilst foregoing the additional efficiencies and safety features that fixed imaging systems and hybrid
1541 suites afford, such as increased heat capacity, precise C arm movements, sophisticated overlay
1542 reference imaging and the ability to perform CBCT immediately following stent implantation.^{221, 222}

1543

1544 5.10.2 Fixed C arms and hybrid suites

1545 Endovascular surgery, defined as endovascular procedures typically performed by vascular surgeons
1546 in an operating room environment, has evolved from relatively simple procedures performed in
1547 traditional operating rooms using mobile C arms, to more complex procedures in dedicated facilities

with fixed C arms. A Hybrid Operating Room is an advanced procedural space that combines a traditional operating room with an interventional suite that incorporates a fixed C arm along with a fluoroscopy capable surgical bed. These Xray machines are more powerful, operating at higher energies with larger beam sizes and detectors which can emit a 3 - 10 fold higher procedural radiation dose compared with mobile C arms.^{141, 224} Similar reductions have been reported during EVAR and TEVAR when moving from a mobile C arm to fixed systems.^{57, 225} In a systematic review to identify studies reporting dose data during EVAR and complex abdominal aortic endovascular repair (F/BEVAR), the lowest DAP levels were identified in modern hybrid rooms with fixed systems.²²⁶ Fixed systems facilitate installation of ceiling and bed mounted lead shielding that in turn protects the operator from radiation exposure.²²⁷ Operators must, however, ensure that they use the lowest image quality feasible as the highest quality images produced by fixed systems are not always necessary and will increase radiation dosage associated with procedure.^{220, 223, 224} It is important to be familiar with and have the situational awareness to continuously employ all the radiation reducing capabilities that a hybrid suite has to offer, in order to offset the increased exposure that accompanies superior imaging.

Recommendation 23	Class	Level	References
An endovascular operating room with a fixed imaging system should be considered in preference to a mobile system for endovascular procedures to improve imaging quality and reduce radiation exposure.	Ila	C	Hertault et al. (2020), ²²⁶ Rehman et al. (2019), ²²⁵ McAnelly et al. (2017), ²²⁸ Zoli et al. (2012) ⁵⁷

5.10.3 Operator Controlled Imaging Parameters

Endovascular therapists working in a hybrid suite can use tableside operator controlled imaging. This ownership of control may reduce unnecessary exposures by avoiding misunderstanding between the operator and another individual tasked with operating the C arm who may misinterpret instructions by the former.²¹⁹ Discrepancies in language, ambiguous words and misinterpretations of commands to move the C arm into a specific position can all lead to unnecessary radiation exposures.²²⁹ Just one study comparing radiographer controlled with operator controlled imaging during EVAR has concluded that median DAP is 30% lower when the operator is in control of the pedal.²³⁰ Further data are, however, required to determine whether operator controlled fluoroscopy can reduce radiation exposure to the operator and patient. In the absence of operator control, clear and unambiguous communication between operator and individual operating the C arm can significantly reduce the time taken to move the C arm and unnecessary radiation exposure.²³¹

Recommendation 24	Class	Level	References
Operator controlled imaging should be considered in preference to tasking another individual, for example radiographer or radiation technologist, with imaging control to reduce radiation exposure during endovascular procedures	IIa	C	Peach et al. (2012) ²³⁰

5.11 Positioning around the patient

5.11.1 Imaging Chain Geometry

Imaging chain geometry describes the linear arrangement between (i) the Xray source and the patient and (ii) the patient and the detector (Figure 10). These distances have a profound independent effect on radiation scatter. The distance between the Xray source and the patient is set by the table height, with the Xray machine's position under the patient, ensuring maximum scatter occurs under the table away from the operator's head and trunk.¹⁴⁷ Although maximising table height from the Xray source will reduce the patient's dose,^{147, 151, 160} this occurs at the cost of significantly increasing scatter to the operator's head, eyes and neck.^{151, 176} The table position needs to be a reasonable distance from the detector, whilst ensuring also that the operator's chest and head is as far away from the patient as possible, as the patient's body is the main source of radiation scatter.¹³⁸ Maximum scatter occurs approximately 1.5m from the floor, this being of particular importance for endovascular therapists of short stature whose upper body are more exposed, making protection measures such as 'stepping back' during DSA vitally important.¹⁵⁰ In these situations, appropriate standing stools may be required to reduce exposure.

The second component of imaging chain geometry is the distance from the patient to the detector, which should be minimal.^{147, 160} Added distance causes dispersion of the Xray beam and a consequential reduction in signal reaching the detector, with a compensatory dose increase initiated by the machine's automatic brightness control.^{138, 145} Reducing the patient to detector distance has several benefits: (i) reduces the energy required to produce the image, thereby reducing scatter (ii) increases scatter absorption by the detector itself and (iii) produces a sharper image.^{148, 176}

1602

1603


1604

1605

1606 Figure 10: Effect of the relative positions of the detector to table on radiation dose measured by Air
1607 Kerma. Whilst the low detector / high table position is best for skin dose, the highest table position
1608 will actually lead to increased scatter to the operator's head and chest, and therefore isn't necessarily
1609 the optimal position for the operator. A balance needs to exist between patient skin exposures and
1610 operator exposure. When different positioning results in equal Air Karma levels, the optimal position
1611 which reduces the operator exposure is typically selected. The optimal position (low detector/high
1612 table) is highlighted in green frame (**).


1613

High Detector / Low Table

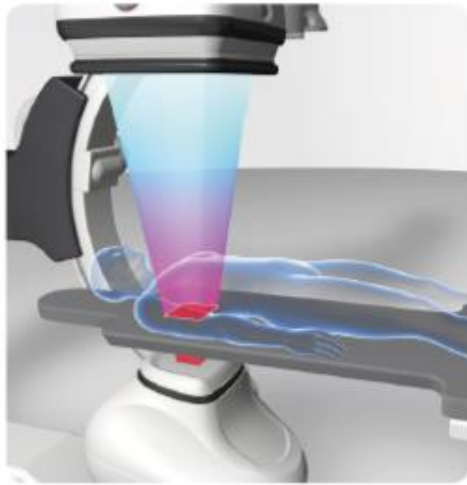

Air Kerma at patient skin

Low Detector / High Table

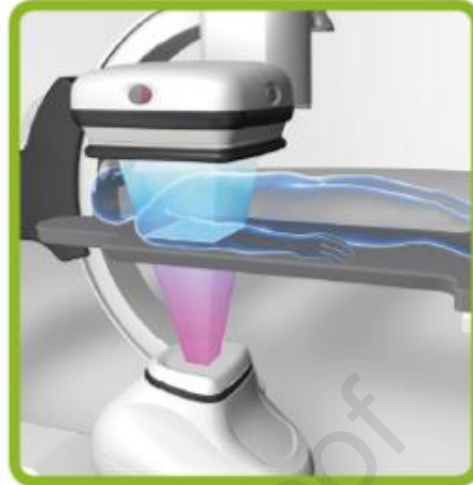


Air Kerma at patient skin

Low Detector / Low Table



Air Kerma at patient skin

High Detector / High Table

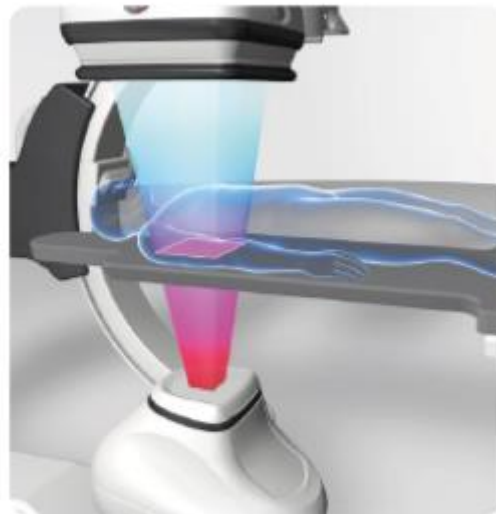

Air Kerma at patient skin

Recommendation 25	Class	Level	References*
Positioning the patient as close as possible to the detector is recommended during endovascular procedures to improve imaging quality and reduce radiation exposure.	I	B	Durán et al. (2013), ¹⁴⁷ Haqqani et al. (2013) ¹⁷¹ *Physics principle



5.11.2 Gantry Angulation


Good imaging chain geometry is complemented by appreciation of the negative influence of angled C arm or gantry positions on radiation dose. Steep C arm angulations (lateral, cranial and caudal) increase radiation dose for several reasons: (i) steeper angles require the Xray machine to emit higher amounts of radiation to achieve the tissue penetration required to produce the same quality image i.e. there is an increase in the thickness of tissue crossed by the beam (ii) this in turn creates more scatter towards the upper body of the operator, increasing exponentially with lateral angulation over 30 degrees and cranial angulation exceeding 15 degrees,¹³⁸ reaching a maximum at full lateral projection;¹⁶⁵ and (iii) steeper angles place the Xray source closer to the patient increasing skin dose and deterministic injury risk, one study reporting 83% of all radiation skin injuries occurring with steep angulation.^{111, 139, 145, 150,}

¹⁷¹ It is advisable that whenever possible, the operators should maintain maximum distance from the radiation source.

On a phantom model, AP projections resulted in 5mSv/hr operator exposure increasing to 11mSv/hr at a 45 degree projection, and 69mSv/hr at 90 degrees.¹⁷¹ Steep angulation such as that required during complex aortic repairs result in significantly higher scatter to the operator, particularly at head level,¹²⁰ with operator radiation exposure being six times higher if they are on the same side as the Xray source (Figure 11).⁶² Cranial left anterior oblique projections cause the most exposure^{6, 120, 147, 160, 165, 232} because the radiation source is usually on the same side as the operator in this configuration leading to maximum backscatter towards the operator.^{165, 176} If possible, the Xray beam should always be positioned on the opposite side from the endovascular operator.

In prolonged cases, frequent alterations in gantry angulation have been recommended in order to reduce skin dose,^{112, 146, 233} but steep cranial and lateral angles should never be used for this purpose.²³³ In obese patients steep angulation compounds the risks and should be used very sparingly.^{26, 145} When steep angulation is essential, it should be used for the shortest period of time with adequate collimation applied.¹³⁸

Figure 11. Angulation of the gantry from AP position (A) to oblique (B) results in almost doubling of radiation dose, measured by DAP, from 34 Gy cm^2 to 66 Gy cm^2 for an equivalent screening time.

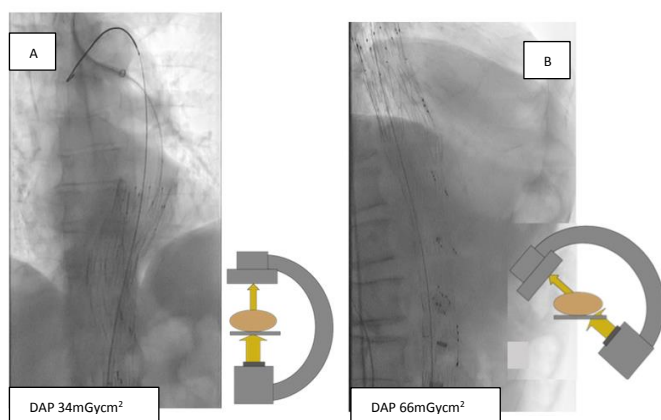

Recommendation 26	Class	Level	References*
Prolonged use of steep gantry angulation is not recommended during endovascular procedures.	III	B	Durán et al (2013), ¹⁴⁷ Haqqani et al. (2013) ¹⁷¹ *Physics principle

1654

1655 5.11.3 The Inverse Square Law and Stepping Away

1656 Scatter radiation comprises the main source of radiation exposure to staff, and by minimising patient
1657 dose, scatter consequently is reduced. However further steps can be taken to reduce exposure to
1658 scatter, the most fundamental is to observe the inverse square law ($X = 1/d^2$, X = exposure, d =
1659 distance). As scatter exits and moves away from the patient there is an exponential reduction in the
1660 number of photons per unit area, and hence potentially harmful ionising energy. Doubling the distance
1661 from the patient quarters exposure and tripling distance reduces it nine fold. This simple but highly
1662 effective act of stepping away from the patient during DSA can considerably reduce personal radiation
1663 dose and is a cornerstone technique to lower exposure.^{7, 145, 147, 165, 173, 176} If there is no need to be in
1664 close proximity to the Xray source or patient, particularly during high dose acquisitions (DSA runs),
1665 then staff should step away as far away as is practical or even exit the room.¹⁶⁵ Indeed it has been
1666 suggested that this should be mandatory behaviour if it does not compromise the safety of the patient.
1667 A relatively safe distance is considered to be 1 - 2 m,⁷ and at 5 m operator dose is effectively
1668 eliminated.¹⁶⁶ Whenever possible, personnel should aim to increase their distance from the radiation
1669 source because even moving away by a small distance can have a substantial effect on the amount of
1670 exposure. Standing closer to the feet of the patient rather than the abdomen during pelvic
1671 interventions has also been shown to be beneficial.¹⁷²

1672

5.11.4 Positioning around the Table

The highest intensity of scatter is located on the Xray beam entrance side of the patient,¹⁴⁷ usually under the table or in left anterior oblique (LAO) projections with the operator standing on the right of the patient. Generally, doses are much higher for primary operators compared with assistants and scrub nurses.^{114, 165} During complex aortic repairs the principal operator can receive twice the dose of the first assistant standing next to them.⁵ The person standing at the opposite side of the table, typically the second assistant standing at the patient's left groin or arm, will receive the next highest dose. The third assistant and scrub nurse position receives undetectable levels for most cases. Linked to gantry position, the variable radiation dose received at different table positions is due to an asymmetric scatter cloud created by interaction of scatter with the complex infrastructure of an angiographic table. Rather than scatter decreasing in predictable concentric circles according to the inverse square law, which governs radiation behaviour in a vacuum, non-conforming patterns of scatter are created around the table.¹⁷⁶ Lateral projections were associated with seven times higher exposure than 45 degree projections, with maximum exposure at the operator and assistant positions if on the same side as the emitter.¹⁷¹ Whilst this should in no way derogate the advice to step away whenever possible, it emphasises the need to move personnel away from the patient when standing on the emitter side of the table during DSA runs, as this is where the highest radiation doses are observed. It is vital to also convey this message to anaesthetic colleagues who are often at the head of the table and close to the source and may even receive significantly higher radiation doses than the primary operator.⁷

The importance of replacing hand injections with remote contrast injectors to reduce interventionists' radiation exposure during Xray guided procedures was highlighted some 40 years ago.²³⁴⁻²³⁶ For most endovascular procedures the working distance from the arterial access site (most commonly the femoral artery) to the area of interest is fixed.¹⁴⁸ For operators who routinely hand inject DSA runs, this accounts for 75% of their total radiation exposure,¹⁶⁶ and 90% of their hand and eye exposure.²³⁶

1698 However this distance can be extended using both power injectors for DSA runs, and extension tubing
 1699 attached to catheters or sheaths for manual injections,^{148, 237} allowing operators to use the inverse
 1700 square law to reduce exposure. The use of power injectors is recommended where feasible,^{7, 147} and
 1701 has been associated with a 50% reduction in operator radiation dose,²³⁸ but must be activated at a
 1702 distance to gain this benefit.

1703

Recommendation 27	Class	Level	References*
The use of power injectors for digital subtraction angiography (DSA) is recommended whenever feasible to reduce radiation exposure to the operator during endovascular procedures.	I	B	Oi (1982), ²³⁴ Goss et al. (1989), ²³⁵ Santen et al. (1975), ²³⁶ Durán et al. (2013), ¹⁴⁷ Mohapatra et al. (2013), ⁷ Larsen et al. (2012) ²³⁸ *Physics principle
Recommendation 28	Class	Level	References*
The distance from the patient to the operator and all other staff should be maximised whenever possible during endovascular procedures.	I	B	Durán et al. (2013), ¹⁴⁷ Haqqani et al. (2013), ¹⁷¹ Mohapatra et al. (2013), ⁷ Kirkwood et al. (2015), ⁵ Larsen et al. (2012), ²³⁸ Patel et al. (2013), ¹⁶⁵ Bacchim et al. (2016) ¹¹⁴ *Physics principle

1705

1706 Chapter 6. Radiation protection equipment in the endovascular

1707 operating room

1708 6.1 Introduction

1709 The majority of studies investigating the effectiveness of radiation shields focus on procedures
1710 performed by cardiologists. These studies are, nevertheless, relevant also for the vascular surgical
1711 setting as most involve femoral access with requirements for both abdominal and chest screening.
1712 Numerous studies have also used phantoms to simulate radiation exposure.

1713 Passive shields can be divided in personal protective devices and shields positioned between the
1714 personnel and the patient (source of scatter). The passive shields are complementary to each other
1715 and to other measures in reducing radiation. Operator refers to the main operator and assistants
1716 refers to the rest of the scrubbed personnel.

1717 There are three types of radiation shielding material.

1718 The first and most well known radiation shielding material is standard lead. Manufactured with 100%
1719 lead, standard lead Xray aprons are the heaviest Xray aprons available. The weight of the apron will
1720 increase depending on the level and areas of protection required, and standard lead Xray aprons are
1721 well suited for shorter procedures.

1722 The second radiation shielding material is a lead based composite; lead composite Xray aprons use a
1723 mixture of lead and other light weight radiation attenuating metals, reducing the weight by up to
1724 25% compared with standard lead aprons. The third option is the total lead free apron (LFA) made of
1725 a blend of attenuating heavy metals other than lead (Pb), which is a lightweight (40% lighter than
1726 standard lead aprons) and non-toxic alternative to the traditional lead apron.

1727 Non-Lead or Lead free Xray aprons are manufactured from a proprietary blend of attenuating heavy
1728 metals, including barium, aluminium, tin, bismuth, tungsten and titanium.

1729 Radiation safety is multidisciplinary, with a key player in achieving a safe environment being the
1730 medical physicist.²³⁹

1731 6.2 Personal protection devices

1732 6.2.1 Wearable aprons

1733 Lead aprons effectively lower the radiation exposure by > 90% to the operator and as such are
1734 adopted as standard safety practice in the endovascular operating room.²⁴⁰ A lead apron with 0.35
1735 mm lead thickness equivalence should be sufficient for most Xray guided procedures. For workload
1736 involving high radiation exposures (Category A workers, see Chapter 3) a wrap around lead apron
1737 with 0.25 mm lead equivalence that overlaps on the front and provides $0.25 + 0.25 = 0.5$ mm lead
1738 equivalence on the front and 0.25 mm on the back is ideal.^{241, 242}

1739 The apron fit is important, especially in the axillary area under the arms since large gaps could
1740 introduce an increased exposure to breast tissue, which is relevant in female staff.¹⁵ Breast cancer
1741 prevalence was reportedly higher among female orthopaedic surgeons compared with U.S.
1742 women.²⁴³ The most common breast cancer site, the upper outer quadrant, may not be adequately
1743 shielded from intra-operative radiation, especially in a C arm lateral projection.^{244, 245} Adding lead
1744 sleeves, wings, and/or axillary supplements at the top of the lead apron may overcome this problem
1745 and should be considered in female operators (Figure 12).²⁴⁵

1746



Figure 12: Operator wearing additional axillary lead protection

The additional weight of the apron places staff at a risk of developing back problems.²⁴⁶ Back pain was reported by 50 - 75% of interventional physicians compare with 27% in a general adult population in the United States.²⁴⁷ A two piece lead garment may shift some of the weight from the shoulders to the hips. Newer generation protective aprons are made from lead composite or lead free materials resulting in a significant weight reduction while, allegedly, maintaining protection that is equivalent to that provided by lead garments.

It is not necessary to use additional lead aprons for the pregnant operator and in fact this is most likely counter productive due to the physical weight. Some facilities will have a maternity apron available which may be more comfortable, particularly towards the latter stages of pregnancy.

The apron lead equivalence requires validation before use.²⁴⁸ Although several studies have shown the safety of lead free aprons²⁴⁹⁻²⁵¹ other studies of both lead containing and non-lead composite aprons have demonstrated wide variations in attenuation of scatter radiation and that they often

1762 provide significantly less radiation protection than manufacturer stated lead equivalence, even in the
 1763 absence of significant defects in the apron when scanned.²⁵²⁻²⁵⁶ In one report some lightweight
 1764 aprons demonstrated significant tears along the seams, leaving large gaps in protection.²⁵³

1765 Aprons should be quality checked annually for any defects to ensure that no cracks in the radio
 1766 protective layer are forming that will allow radiation through to the wearer. This includes visual and
 1767 tactile inspections for tears, kinks and irregularities, and an evaluation of the extent of damage to the
 1768 internal radiation shields via fluoroscopy, under the guidance of a medical physicist.²⁵⁷ Aprons must
 1769 be handled carefully, never be folded or creased, and stored safely on purpose designed lead apron
 1770 racks to ensure that the integrity of the shielding material remains intact. Cleaning is done with a
 1771 damp cloth using only cold water and mild detergent.²⁵⁸⁻²⁶⁰

1772 A recent paper reported a 63% incidence of free lead on the surface of lead aprons and this was
 1773 associated with the visual appearance of the apron, type of shield, and storage method.²⁶¹ Lead
 1774 exposure from free surface lead represents a potentially serious and previously unknown
 1775 occupational safety issue. Further studies of this risk are warranted.

1776

Recommendation 29	Class	Level	References*
All personnel in the endovascular operating room are recommended to always wear a well fitting protective apron with at least 0.35 mm of lead thickness equivalence	I	B	Badawy et al. (2016), ²⁴⁰ NRCP report No. 168 (2010) ¹⁵ *Physics principle
Recommendation 30			

The use of axillary supplements and or sleeves to improve protection of the breast should be considered for female operators	Ila	C	Van Nortwick et al. (2021), ²⁴⁵ Valone et al. (2016) ²⁴⁴
Recommendation 31			
Protective shielding and personal protection equipment are recommended to be checked for lead equivalence and integrity by a medical physicist, before being used for the first time and then on an annual basis	I	B	Oyar et al. (2012), ²⁵⁹ Burns et al. (2017), ²⁶¹ Finnerty et al. (2005), ²⁵² Fakhoury et al. (2019), ²⁵³ Lu et al. (2019) ²⁵⁴ *Physics principle

1777

1778

1779 6.2.2 Thyroid Collar

1780 The thyroid is a radiosensitive organ and has been linked to an increased risk of carcinogenesis from

1781 external ionising radiation.²⁶² However, these results are limited by the age range in these studies,

1782 with limited risk seen after exposure beyond the age of 20 years. Nevertheless, the thyroid of the

1783 operator will receive significant scattered radiation if unprotected. A thyroid collar also provides

1784 protection for other neck organs, such as the thymus and the carotids, although the value of this is

1785 not clear. Consequently, a thyroid collar should always be worn and attention should be paid to

1786 minimising any gaps between the thyroid shield and the lead apron.^{9, 15} Thyroid collars should also be

1787 quality checked annually.

1788

Recommendation 32	Class	Level	References
All personnel in the endovascular operating room are recommended to always wear thyroid collars	I	C	Ron et al. (1995), ²⁶² NRCP report No. 168 (2010), ¹⁵ ICRP publication 139 (2018) ⁹

1789

1790 6.2.3 Leg shields

1791 A recent study demonstrated DNA damage to the operators performing EVAR procedures which was
 1792 abrogated by leg shielding.⁶ Although the under table protective drapes should attenuate scatter
 1793 reaching the lower extremities of the operator that are not shielded by the standard lead apron in
 1794 most situations, additional protection with leg or tibial shields should be considered in high dose
 1795 environments. Measurements of leg doses have been found to be as high as 2.6 mSv per procedure
 1796 in interventional radiologists when shielding is not used.²⁶³

1797

Recommendation 33	Class	Level	References
Endovascular operators should consider using leg shields in addition to table mounted skirts	IIa	C	El-Sayed et al. (2017), ⁶ Whitby et al. (2003) ²⁶³

1798

1799 6.2.4 Glasses and visors

1800 The main effect of ionising radiation on the eyes is the onset of posterior cortical and subcapsular
 1801 cataracts, radiation induced cataract (RIC). Recent studies suggest that RIC shares some common
 1802 mechanisms with carcinogenesis and may form stochastically, without a threshold and at low
 1803 radiation doses.²⁶⁴⁻²⁶⁸

1804 The endovascular operator can potentially receive annual eye doses above 20 mSv/year and there
 1805 are several retrospective studies of operators carrying out Xray guided procedures having a higher
 1806 prevalence of lens changes that may be attributable to ionising radiation exposure. While most of
 1807 these changes are subclinical, they are important due to the potential to progress to clinical
 1808 symptoms, highlighting the importance of minimizing staff radiation exposure.^{79, 80, 269, 270}
 1809 Consequently, the need for protective measures for the eyes is evident.

1810 There are several protective eyewear with transparent lead glass screen available; eyeglasses with or
 1811 without individualised prescription glasses, fit over glasses with space for personal eyeglasses under,
 1812 and visor. Typical lead equivalent thickness of radiation protective eyewear is 0.75mm. Theoretically
 1813 this would result in > 90% attenuation. However, the actual lens dose is higher due to exposure from
 1814 the side, below, and backscatter from head.

1815 Although use of lead eyewear efficiently reduces scatter radiation to the operator's eyes in daily
 1816 practice,²⁷¹ the protection with different eyewear is far from perfect and varies substantially
 1817 depending not only on the eyewear and its fitting to the face but also with the variation of radiation
 1818 geometry depending on the imaging projections used. To be effective, glasses should have a good
 1819 tight fit, as any gaps can significantly affect its protective ability. Scattered radiation penetrates from
 1820 the side and glasses with side shields should be considered preferentially.²⁷²

1821 Secondly scattered radiation from the operator's head contributes significantly to ocular exposure.
 1822 Optimal radiation protection of the eyes during Xray guidance thus depends not only on eyeglasses
 1823 with leaded glass, but also on shielding of sufficient size and shape to reduce exposure to the
 1824 surrounding head.²⁷³ Thus, to achieve an adequate protection of the eyes use of a ceiling mounted
 1825 shield is vital and personal protective eyewear should only be seen as complementary.

1826 Although there are no data showing a clinical protective effect of lead eyewear, in the form of a
 1827 reduced frequency of RIC, there is enough indirect evidence to support a strong recommendation

that all operators in the endovascular operating room should wear them at all times and in combination with ceiling mounted shields. (See 6.3.2 Recommendation 32).

The risk of RIC in non-operators has not been studied and given the inverse square law the risk should be considerably lower in the non-operating individuals in the endovascular operating room. Although it cannot be ruled out that non-operators may also benefit from lead glasses, this group is not included in the recommendation at this time.

Recommendation 34	Class	Level	References*
Endovascular operators are recommended to always wear appropriately fitted lead glasses with at least 0.75 mm of lead equivalence during endovascular procedures	I	B	Karatassakis et al. (2018), ⁸⁰ Matsubara et al. (2020), ²⁶⁹ Elmaraezy et al. (2017), ⁷⁹ Bitarafan Rajabi et al. (2015), ²⁷⁰ Maeder et al. (2006) ²⁷¹ *Physics principle

6.2.5 Hand shields

The hand receives a significant amount of radiation (up to 1.5 mSv per procedure, or 50 mSv per year) during procedures since it is unshielded and close to the radiation source.^{15, 274} However, this level of exposure is unlikely to have any adverse health impact.

Leaded gloves are available but are bulky, stiff and heavy and cannot be used when dexterity is required. The introduction of leaded (or lead free) radiation attenuating latex gloves helps address these issues. These gloves can shield the hand by 15 - 30%.^{275, 276}

However, if the hand with an attenuating glove is placed in the direct radiation beam then the dose to both the patient and operator will increase because the automatic exposure control system in current Xray systems will boost the radiation output.²⁴⁰

Thus, the best method to protect the hands is to keep them away from the primary beam, and consequently, radiation protection gloves are rarely needed and are not recommended in routine clinical practice. In cases where the hands must be close to the patient such as during an Xray guided vascular puncture, protective gloves may be an option. However, for many reasons also in addition to radiation safety, routine use of an ultrasound guided puncture technique, rather than a fluoroscopy assisted puncture, is recommended,²⁷⁷⁻²⁸⁰ and when that is not feasible procedure modifications such as using a long needle or syringe to extend the working length of a needle may be preferable. When gloves are used, single use, non-lead radio protective gloves are recommended since they can be safely disposed of after a procedure unlike a leaded glove.

Recommendation 35	Class	Level	References*
Routine use of an ultrasound guided artery puncture technique, rather than fluoroscopy assisted puncture, is recommended to reduce radiation exposure to the hand.	I	B	Seto et al. (2010), ²⁷⁷ Slattery et al. (2015), ²⁷⁸ Sobolev et al. (2015), ²⁷⁹ Stone et al. (2020) ²⁸⁰ *Physics principle

Recommendation 36	Class	Level	References
Routine use of radiation protective gloves is not recommended during endovascular procedures	III	C	Badawy et al. (2016) ²⁴⁰

1860

1861 6.2.6 Head shields

1862 Reports regarding operator brain tumours associated with Xray guided procedures have raised
 1863 concerns regarding appropriate shielding to the head.^{72, 281, 282} However, a true increased risk of brain
 1864 tumours among physicians performing interventional procedures has not been established.

1865 Older generations of lead caps, with 0.5 mm lead, effectively lower the exposure to the head.^{283, 284}

1866 However, the average weight of these caps is > 1 kg, which may be uncomfortable to wear and could
 1867 present a musculoskeletal occupational health and safety hazard in itself .

1868 The reported radioprotection efficacy of newer generation lightweight lead free (bismuth oxide
 1869 composite) caps varies considerably. Some suggest them to provide significant radiation protection
 1870 to the head, similar to standard 0.5 mm lead equivalent caps,^{71, 285-289} while others found only
 1871 negligible exposure reduction.²⁹⁰⁻²⁹² The different results may depend on how the measurements
 1872 were made. In a phantom model study a small but significant attenuation superficially on the skull,
 1873 but no reduction in dose for the middle brain, was found. This was suggested to be explained by the
 1874 fact that the majority of radiation to an operator's brain originates from scatter radiation from angles
 1875 not shadowed by the cap, and the authors concluded that radiation protective caps have minimal
 1876 clinical relevance.²⁹²

1877 Thus, whether radioprotective caps actually provide dose reduction to the brain is disputed, and
 1878 more importantly, whether they prevent radiation induced damage is completely unknown. Based on
 1879 current evidence they are therefore not recommended in routine clinical practice. It is more effective

to use the ceiling shield.²⁹³ However, in vascular procedures that are likely to give rise to high operator dose, consideration may be given to wearing them. There is evidence to suggest that dose to the head is lower in operators taller than 180cm in height, with a decrease in dose to the head of 1% per cm of operator height above 180cm.²⁸³ Hence, these caps may be of greater benefit in operators of shorter height.

Alternative and better head protection equipment is discussed below (See 6.3.1 Recommendation 21).

Recommendation 37	Class	Level	References
Use of radiation protective head caps is not indicated in routine clinical practice,	III	C	Fetterly et al. (2017), ²⁹⁰ Sans Merce et al. (2016), ²⁹¹ Kirkwood et al. (2018), ²⁹² Fetterly et al. (2011) ²⁹³

In summary, the endovascular operator should always wear an apron, thyroid collar, and lead glasses (Figure 13). In addition, one should consider leg shields, but refrain from gloves and cap.



1891

1892 Figure 13. As minimum protection, an endovascular operator should always wear a lead apron,
1893 thyroid collar and fit over lead glasses

1894 6.3 Other radiation shielding equipment

1895 6.3.1 Suspended personal radiation protection systems

1896 The suspended personal radiation protection system was designed to enhance radiation protection
1897 and at the same time improve ergonomics and comfort by eliminating weight on the operator, while
1898 maintaining a neutral or positive effect on task accomplishment. The Zero-Gravity suspended
1899 radiation protection system is currently the only commercially available system (Figure 14). It has a
1900 full body 1.25 mm lead apron and 0.5 mm lead equivalent face and head shield.²⁹⁴



Figure 14. A suspended personal radiation protection suit

Compared with a conventional lead apron, the Zero-Gravity Suit system provided a 16 to 78 fold decrease in radiation exposure for a sham operator in a simulated clinical setting.²⁹⁴ In a clinical study by Savage et al. the Zero-Gravity Suit provided superior operator protection during Xray guided procedures compared with conventional lead aprons in combination with standard shields. Exposure to the eye, head, humerus, torso, tibia and back was reduced by 88 - 100% with undetectable or barely detectable radiation doses with the Zero-Gravity Suit. The Zero-Gravity Suit was furthermore regarded as more comfortable, with relief of back pain, and considered less obstructive relative to a standard lead apron and shields by the operators.²⁹⁵ In a small study, the overall accumulated dose for the operator was four times higher for standard protection devices vs. the Zero-Gravity Suit. However, some exposure still occurred at the level of the lens and thyroid and the authors concluded that although the Zero-Gravity Suit leads to substantially lower radiation exposure to the operator additional protection is justified.²⁹⁶ In a single operator the annual body and eye dose was reduced by 70 - 87% and 16 - 60%, respectively, after the introduction of a Zero-Gravity Suit system.²⁹⁷ Compared with conventional lead aprons the use of suspended lead during percutaneous coronary intervention was associated with significantly less radiation exposure to the chest (0.0 μ Sv vs. 0.4

1919 μSv , $p < .00$) and head ($0.5 \mu\text{Sv}$ vs. $14.9 \mu\text{Sv}$, $p < .001$)²⁹⁸ and a 94% reduction in head level physician
 1920 radiation dose.²⁹⁹

1921 Although traditional personal protective equipment, when used together with other shields, provide
 1922 comprehensive radiation protection, there are limitations, especially regarding scattered radiation to
 1923 the head, eyes and lower legs. Given the demonstrated superior protective effect to the whole body
 1924 by the Zero-Gravity Suit it is justified to consider the system in high dose environments.

1925 The full body suspended radiation protection system usually replaces the traditional personal
 1926 protective equipment (i.e., lead apron, thyroid shield, and shin guards) while personal protective
 1927 glasses can still be worn. The use of full body suspended radiation protection systems may reduce
 1928 the possibility to use ceiling mounted standard lead shields, which is suboptimal, and care should be
 1929 taken for its continuous use as a complement to the full body suspended radiation protection
 1930 systems.

1931 The cost can be a potential holdback in acquiring the full body suspended radiation protection
 1932 system, and there is a certain learning curve to get used to the system, by both the operator and the
 1933 staff who will prepare it.

1934

Recommendation 38	Class	Level	References
A full body shield suspended radiation protection system should be considered in high dose endovascular procedures	Ila	C	Marichal et al. (2011), ²⁹⁴ Savage et al. (2013), ²⁹⁵ Haussen et al. (2016), ²⁹⁶ Pierno et al. (2012), ²⁹⁷ Madder et al. (2017), ²⁹⁸ Salcido-Rios et al. (2021) ²⁹⁹


1935

6.3.2 Radiation protective shielding above and below the table

Radiation protective shielding can be mounted on the ceiling, on the operating table or mobile on wheels. Ceiling mounted lead acrylic shields are common and their importance cannot be over emphasised (see figure 15). Proper use of these shields can significantly lower the radiation dose to the operator's head and neck.^{271, 293, 300, 301} The protection conferred to the operator is substantially compromised if these shields are not correctly positioned and must be adjusted as the table and C arm position and C arm angle changes during the case prior to fluoroscopy and digital subtraction angiography. If the ceiling mounted shielding is placed closer to the patient, a larger solid angle is shielded but with lower efficiency. On the other hand, if the shielding is placed close to the operator, a smaller solid angle is shielded but with higher efficiency. This should be taken into account when more people are present in the operating room, as is often the case during endovascular procedures.³⁰² The shield is most effective for providing upper body protection during right femoral access procedures when it is positioned just cephalad to the access site and is tight to the anterior and right surfaces of the patient. A shield positioned 20cm away from the groin results in twice the scatter radiation than if it placed closer to the access site; in addition to this, a 5 cm gap between the shield and the patient's body results in a further four fold increase in operator exposure²⁹³ It is important to note that, although ceiling mounted shields reduce operator eye exposure by a factor of 19, they have minimal benefit on reducing radiation exposure to the hands and further measures must be taken.²⁷¹

Figure 15: Shielding around the endovascular operating table (A) showing mobile anaesthetic protection shield (triangle), table mounted lower shield (arrow) and bilateral ceiling mounted upper shields (A asterix) and their optimal positioning (B asterix).

1960

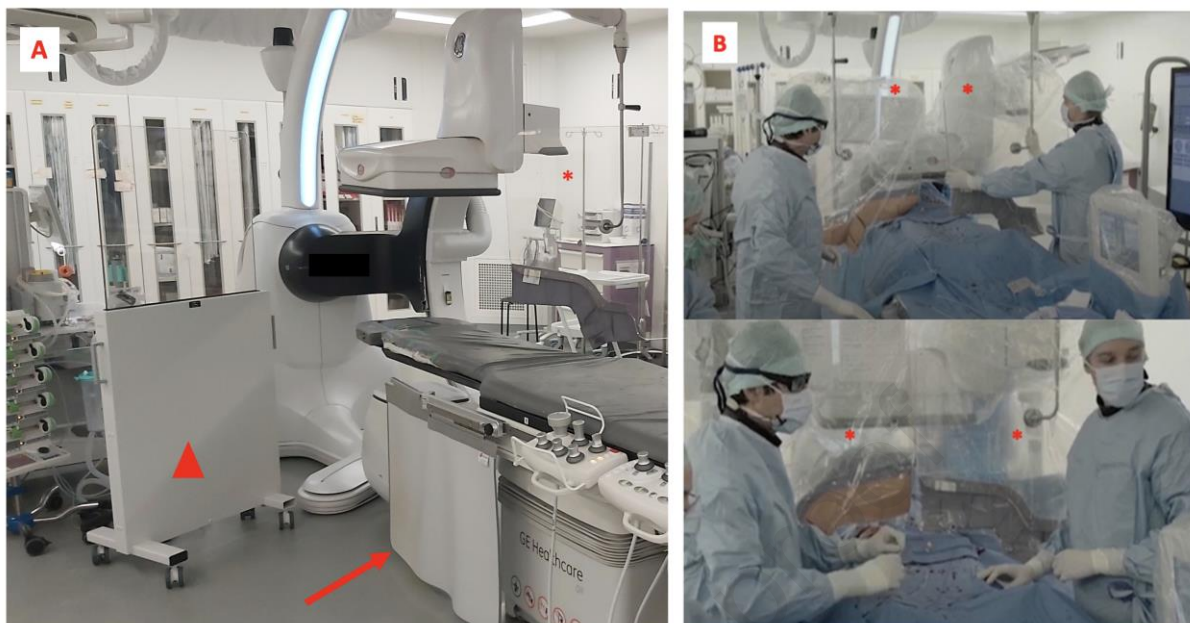

1961

1962

1963 Phantom studies have shown that larger shields with patient contour cutout that allow the curved
 1964 gap to adapt to the patient's body, along with a flexible curtain below the shield that is in contact
 1965 with the patient's body, reduces the dose to the operator by up to 87.5% compared with a bare
 1966 shield. These soft extensions along the bottom edge maintain contact between the patient and shield
 1967 to reduce the amount of scatter directed towards the operator. This configuration provides better
 1968 protection to the heads of tall operators and achieves similar magnitudes of dose reduction for the
 1969 assistant.³⁰³ Other shielding such as table mounted vertical side shields should also be considered;
 1970 these can be removed easily if imaging is hampered during steep C arm angulation.

1971 Although the majority of energy from Xrays is deflected upward and absorbed by the patient's body,
 1972 the downward energy does not encounter such a barrier without shielding. As a result, radiation
 1973 doses are high at the operator's legs; measurements of leg doses have been found to be as high as
 1974 2.6 mSv per procedure in interventional radiologists when shielding is not used.²⁶³ Adequate
 1975 shielding from the Xray beam placed under the operating table during endovascular procedures is,

therefore, essential for protection against scattered radiation. Table mounted lead skirts, usually in the form of leaded slats hanging from the side of the table and close to the floor, are highly recommended. As they are flexible (and can be swung 90 degrees horizontally when needed), lead skirts can be adopted for the majority of endovascular procedures as they can accommodate a range of C arm angles. Although wearable aprons provide the majority of the shielding, table lead skirts do decrease the radiation dose even further by over 90%²⁹³ and their adjunctive use for protection under the operating table results in a significantly lower radiation dose to the operator's pelvis and thorax.³⁰⁴ Phantom studies have shown that when ceiling suspended lead screens are combined with table mounted shielding, operator and assistant radiation exposure is reduced by up to 90%.³⁰⁵

Other members of the team, including the anaesthetist and nursing staff must be protected from radiation. This can be readily achieved by using floor standing mobile accessory lead shields that have an effective lead thickness of 0.5mm. These can reduce radiation exposure to other members of the team by over 60%.³⁰⁶

Recommendation 39	Class	Level	References*
All operators are recommended to use ceiling mounted shields as first line protection at all times during endovascular procedures	I	B	Fetterly et al. (2011), ²⁹³ Maeder et al. (2006), ²⁷¹ Thornton et al. (2010), ³⁰⁰ Eder et al. (2015) ³⁰³ *Physics principle
Recommendation 40			

All operators are recommended to use table mounted lead skirts as first line protection at all time during endovascular procedures	I	B	Whitby et al. (2003), ²⁶³ Fetterly et al. (2011), ²⁹³ Sciahbasi et al. (2019) ³⁰⁴ *Physics principle
Recommendation 41			
Ceiling and table mounted shields are recommended on both sides of the operating table when personnel exposure is anticipated on both sides	I	B	Jia et al. (2017) ³⁰⁵ *Physics principle

1990

1991 6.3.3 Radiation protective patient drapes

1992 Radioprotective sterile drapes include covered non-lead sheets or drapes that are made of bismuth

1993 or tungsten antimony. They are placed on top of the patient to attenuate the scatter radiation that

1994 contributes to operator dose at the source.³⁰⁷ Phantom studies show that these drapes reduce

1995 scatter radiation by a factor of 12, 25 and 29 for the eyes, thyroid and hands respectively compared

1996 with standard surgical drapes.³⁰⁸ The dose reducing function is comparable to approximately 0.4 - 0.8

1997 mm lead. The majority of evidence for these radioprotective drapes has been accumulated in

1998 cardiology procedures, where they have been shown to reduce the scatter radiation dose to the

1999 operator by from 20% to 80%.³⁰⁹⁻³¹³

2000 Although there is a lack of evidence for use of these drapes in endovascular surgery, a single centre

2001 study has shown that their use during infrarenal EVAR results in a dose reduction to the hand and

2002 chest of the operator by 49% and 55% respectively as well as a 48% reduction to the chest of the

2003 theatre scrub nurse.³¹⁴ One other study evaluating the effectiveness of these drapes in lower limb
 2004 endovascular procedures (covering the leg closest to the operator and the chest), reported a
 2005 significant dose reduction rate of 65%.³⁰⁹

2006 Diligent and judicious use of ceiling and table mounted radioprotective shields and drapes is
 2007 recommended for all endovascular procedures. In fact, when these are used in combination with
 2008 other interconnecting flexible radiation resistant materials, it is possible to create an attenuation
 2009 barrier so effective that operator exposure at various sites is barely detectable and approaches
 2010 background levels.³¹⁵

2011 When placing disposable drapes on the patient, attention is required to avoid having the drapes in
 2012 the primary beam, which might increase patient and operator exposure.⁹ The cardiology intervention
 2013 setting, where the operator maintains the same position throughout most of the procedure, may
 2014 differ from the endovascular setting, where the operator often uses multiple positions making the
 2015 use of protective drapes less straightforward. Furthermore, although some studies suggest that the
 2016 observed reduction in dose to the operator can be achieved without increasing the dose to the
 2017 patient³¹⁶ other studies have found that drapes reflect scatter radiation back to the patient thereby
 2018 significantly increasing the radiation dose to the patient.³¹⁷

2019

Recommendation 42	Class	Level	References
Use of radiation protective drapes may be considered during endovascular procedures	IIb	C	Marcusohn et al. (2018), ³⁰⁷ King et al. (2002), ³⁰⁸ Power et al. (2015), ³⁰⁹ Vlastra et al. (2017), ³¹⁰ Ordiales et al. (2017), ³¹¹ Politi et al. (2012), ³¹²

			Simons et al. (2004), ³¹³ Kloeze et al. (2014), ³¹⁴ Musallam et al. (2015) ³¹⁷
--	--	--	--

2020

2021

Journal Pre-proof

Chapter 7. Education and training in radiation protection

7.1 Introduction

Reports suggest an alarming knowledge gap related to the principles of radiation exposure protection among medical professionals, especially trainees, involved in Xray guided procedures. Only 39% of French vascular trainees responded to a survey administered in 2016 and those who responded felt only moderately satisfied with their radiation protection training. The ALARA principle was well known by these responders but basic knowledge about biological risks and radiation physics was poor.¹⁴⁰ In another survey, 45% of vascular surgical trainees in the US, had no formal radiation safety training, 74% were unaware of the radiation safety policy for pregnant women, and 43% did not know the yearly acceptable level of radiation exposure.⁹⁵ Similar results have been shown for trainees in cardiology,³¹⁸ urology³¹⁹, and orthopaedic surgery.^{320, 321} A recent US survey (95 trainees, 27% response rate) revealed that a high number of vascular trainees are exceeding radiation exposure limits. The majority (77.9%) had received formal radiation safety education, but 25% had never received feedback on radiation exposure levels nor had 52% met their radiation safety officer.³²²

Procedures performed by less experienced operators are associated with higher radiation exposure in cardiology,³²³⁻³²⁵ orthopaedic surgery,³²⁶ interventional radiology and neuroradiology.³²⁷ The learning curve in FEVAR may substantially influence operator dose³²⁸ but the evidence on this is contradictory, with some studies reporting no difference in operator dose based on the level of training during complex endovascular procedures.^{5, 165}

A recent European needs assessment for simulation based education in vascular surgery prioritised basic endovascular skills, including radiation safety, as the second most important procedural skill in vascular surgery training.³²⁹ Radiation safety education and training should be a priority not only for vascular surgical trainees but for all personnel in the endovascular operating room, involved in procedures using radiation at every level of training.³³⁰

2046 7.2 Delivery of radiation protection education and training

2047 The primary trainer in radiation protection should be a person who is an expert in radiation safety,
 2048 usually a medical physicist. Input from radiation protection certified clinicians who carry out day to
 2049 day Xray guided work is valuable.^{331, 332}

2050 The training program in radiation protection should be relevant, require a manageable time
 2051 commitment and be oriented towards the clinical practice of the target audience.³³³ These programs
 2052 should include initial basic education for all personnel in the endovascular operating room, and more
 2053 in depth education and training for specialists who use ionising radiation in endovascular procedures.
 2054 Recommendations on the curriculum have been provided by international organisations such as the
 2055 ICRP, the European Commission and the World Health Organisation. An overview of the core
 2056 knowledge that should be included within the radiation protection education and the level of
 2057 knowledge and understanding that every category should obtain, is outlined in these documents.

2058 In 2019, a European survey about radiation protection training was sent out to the European
 2059 Vascular Surgeons in Training (EVST) representatives. Twenty-one of 28 European member states had
 2060 a representative in the EVST council at the time. Two thirds of the countries (14 of the total of 21) are
 2061 obliged to take a mandatory course during their vascular surgery training but only in half of the cases
 2062 is it followed by a post-course evaluation. This mandatory course includes theory (all 14), hands on
 2063 training (4/14) and or web based learning (4/14). The course should be taken during medical school
 2064 (1/14), before being exposed to radiation or using it yourself (5/14) but in most cases only before
 2065 board certification in vascular surgery (8/14). Re-certification is mandatory in half of the countries
 2066 (7/14): yearly (1/14), every two years (3/14), or every five years (3/14). Of the countries where a
 2067 radiation protection course is not mandatory, a voluntary course or training is available in four of
 2068 seven.⁹³

2069

Recommendation 43	Class	Level	References
All personnel who may be exposed to radiation in the endovascular operating room must have had the appropriate level of radiation protection training	I	Law	ICRP publication 105 (2007), ¹³⁷ ICRP publication 113 (2009), ³³⁴ EBSS (2013) ⁸

2070

2071 7.3 Theoretical courses

2072 The majority of radiation protection programmes focus on knowledge training using the traditional
 2073 classroom format, but e-learning or web based courses are being used increasingly.³³⁵⁻³³⁷ The main
 2074 advantages of e-learning include flexibility in time management, easy access to resources, and
 2075 learning at ones own speed but it lacks interaction with teachers and other participants.

2076 A multicentre study has shown that after a practical 90 minute interactive training session (ELICIT,
 2077 Encourage Less Irradiation Cardiac Interventional Techniques) operators use shorter FT, fewer DSA
 2078 runs, consistent collimation and less steep C arm angulations, resulting in a reduction in DAP from
 2079 26.5 to 13.7 Gy.cm² (48.4%).^{208, 338} The patient related dose reductions are consistent and long
 2080 lasting.³³⁹ Focused events on minimising radiation exposure and optimal use of Xray equipment
 2081 during coronary intervention have similarly resulted in dose reductions.³⁴⁰ A systematic review
 2082 suggests that radiation protection training can result in a > 70% reduction in operator dose and an
 2083 almost halving of the patient dose.³⁴¹ The specific instructional courses reviewed included short 90
 2084 min courses and basic and advanced theoretical courses delivered over either 20 hours or 48 hours.
 2085 Implementing a culture of radiation safety, including Xray imaging and radiation safety laboratory
 2086 sessions and a practical examination between 2008 - 2010, led to a 40% reduction in cumulative skin
 2087 dose in the endovascular operating room over three years despite an increased participation of
 2088 fellows in training.³⁴²

2089

2090 7.4 Practical training

2091 Practical exercises and practical sessions are beneficial particularly if carried out in a similar
 2092 environment to that in which the team will be operating.³³³ Availability of practical courses varies
 2093 between European countries but some offer hands on training in credentialed centres as part of their
 2094 training program, ultimately creating a culture of respect for the hazards of radiation.³⁴³ In
 2095 Switzerland, for example, two full days of hands on radiation protection training, including an
 2096 examination is mandatory to obtain board certification in any surgical specialty.³⁴⁴ A curriculum in
 2097 radiation protection for medical practitioners has been established in Spain and the practical aspects
 2098 of training have been well received.³⁴⁵ Some practical simulation sessions are solely web based and
 2099 allow the operator to alter angulation, magnifications, pulse rate and immediately test the influence
 2100 of each factor on the radiation dose and scatter. This type of training allows the operator to put
 2101 knowledge into practice and to reduce radiation doses to patient and operators in the cardiac
 2102 catheterisation laboratory, for example, with an average reduction in the monthly exposure from
 2103 0.58+/-0.14 to 0.51+/-0.16 mSv for some operators.³⁴⁶ Ideally, the radiation safety performances of
 2104 trainees in simulated or real endovascular interventions should be evaluated regularly using a
 2105 reliable rating scale to provide formative feedback.¹⁴²

Recommendation 44	Class	Level	References
The inclusion of radiation protection content in national vascular board certification exams is recommended.	I	C	Consensus

2106

2107 Medical simulators are useful for learning new skills using C arms before applying them to patients.

2108 Practicing endovascular techniques, including iliac angioplasty or stenting, carotid artery stenting and

2109 EVAR on a virtual reality (VR) simulator improves performance on the simulator with a reduction of
 2110 total procedure time and FT during real cases.³⁴⁷⁻³⁵¹ These simulated modules focus on learning
 2111 procedural steps and becoming familiar with new devices. The reduction in FTs may be explained by
 2112 the fact that the operator steps on the fluoroscopy pedal less frequently and for a shorter duration
 2113 most probably because of an improvement in both the hand eye foot coordination and use of
 2114 endovascular tools. It is acknowledged that trainees require 300 coronary angiography cases to
 2115 achieve the proficiency level of consultants³⁵² and if VR training shortens and flattens the learning
 2116 curve, then training in this safe environment may also have an impact on patient and occupational
 2117 radiation dose.

2118 By integrating a medical simulator in a fully immersive simulation training with a complete surgical
 2119 team, the trainee may not only improve his or her technical skills but also enhance the radiation
 2120 safety behaviour of the entire team. Examples include ensuring that the entire endovascular
 2121 operating team is wearing lead and asking the team to step back before DSA runs.³⁵³

2122 Only a few studies have evaluated whether the reduced FT achieved using VR training translates into
 2123 real life procedures. Hands on training using VR simulation for endourology, gastroenterology and
 2124 orthopaedic procedures reduces FT during real life operations.³⁵⁴⁻³⁵⁷ A significant reduction in FT was
 2125 achieved in real life electrophysiology cases after simulator based training and, similarly, a RCT
 2126 assessing the effect of simulation training on diagnostic angiography found a significant reduction in
 2127 FT and radiation dose during the actual coronary angiograms carried out by the group who had had
 2128 simulation training compared with the one that did not.³⁵⁸⁻³⁶⁰ In the peripheral endovascular field,
 2129 few RCTs have shown the transferability of endovascular skills acquired during simulation based
 2130 training to real life with enhancement in the individual measures of performance including the
 2131 awareness of fluoroscopy usage.³⁶¹ In the PROficiency based StePwise Endovascular Curricular
 2132 Training (PROSPECT) study, consisting of e-learning and hands on simulation modules, focusing on
 2133 iliac and superficial femoral artery atherosclerotic disease, those trainees who had access to

simulator based training in addition to knowledge and traditional training outperformed the other groups and showed a trend towards less contrast and radiation use.³⁶² Simulation (VR simulation, augmented reality, 3D printing) is becoming more practical for everyday use and patient specific rehearsals may reduce the radiation exposure during these procedures.³⁶³⁻³⁶⁵ Despite the lack of large RCTs, the benefit of learning and practicing endovascular skills in a safe, radiation free environment, should be acknowledged in reducing the radiation dose in real life endovascular procedures. This is especially important in young visiting persons (trainees, medical or nursing students, and observers) who are sometimes forced or allowed to receive large amounts of radiation while assisting or performing complex endovascular procedures. Therefore, extra care should be taken to avoid excessive radiation exposure to students and visiting persons.

Recommendation 45	Class	Level	References
Simulation based training should be considered to acquire the appropriate technical skills to reduce the amount of radiation during endovascular procedures	Ila	C	Chaer et al. (2006), ³⁶⁶ De Ponti et al. (2012), ³⁵⁹ Prenner et al. (2018), ³⁵⁸ Popovic et al. (2019), ³⁶⁰ Desender et al. (2016) ³⁶³

7.5 Timing of radiation protection education and training

To ensure that continuing education and training after qualification is provided, radiation protection training programs should be updated regularly and re-training should be planned at least every 36 months or when there is a significant change in radiology technique or radiation risk (figure 16).³³⁴

Radiation protection education should be integrated into the curricula of medical, nursing or other schools ensuring the establishment of a core competency in these areas.³⁶⁷ Ideally access to any

facility using radiation should be prohibited until at least core knowledge has been obtained. For future endovascular operators, education and training should continue throughout residency, but especially at the beginning of the endovascular career, to establish a foundation of correct practice early on. This may be accomplished during focused specific courses, but it may also be facilitated by increased interactions and teaching with the personnel in the endovascular operating room. Evaluation and certification are crucial. Modest improvements in radiation use have been noted with a single education event alone, but regular detailed personalised feedback comparing an individual's radiation use to the rest of their local peer group and external benchmarks has a greater impact.³⁶⁸ Regulatory and health authorities can enforce radiation protection training, certification and periodic updates for the personnel in the endovascular operating room⁸ (also see chapter 3). Evidence of certification should ideally be maintained in a central register. A structural chapter about radiation safety and protection should be included in the European Union of Medical Specialists to be recognised as a fellow of the European Board of Vascular Surgery. Scientific societies are ideally placed to support and promote radiation protection training by including lectures on radiation protection and offering refresher courses at scientific congresses.³³³


Recommendation 46	Class	Level	References
National policies regarding continuous training and certification with formal assessment in radiation protection must be followed.	I	Law	ICRP publication 105 (2007), ¹³⁷ ICRP publication 113 (2009) ³³⁴ EBSS (2013), ⁸ Kuon et al. (2005), ³³⁸ Azpiri-Lopez et al. (2013), ³⁴⁰ Kuon et al. (2014) ²⁰⁸

2169

2170 Figure 16: Timeline for radiation protection training and certification for healthcare professionals

2171 suggested by the Guideline Writing Committee.

2172

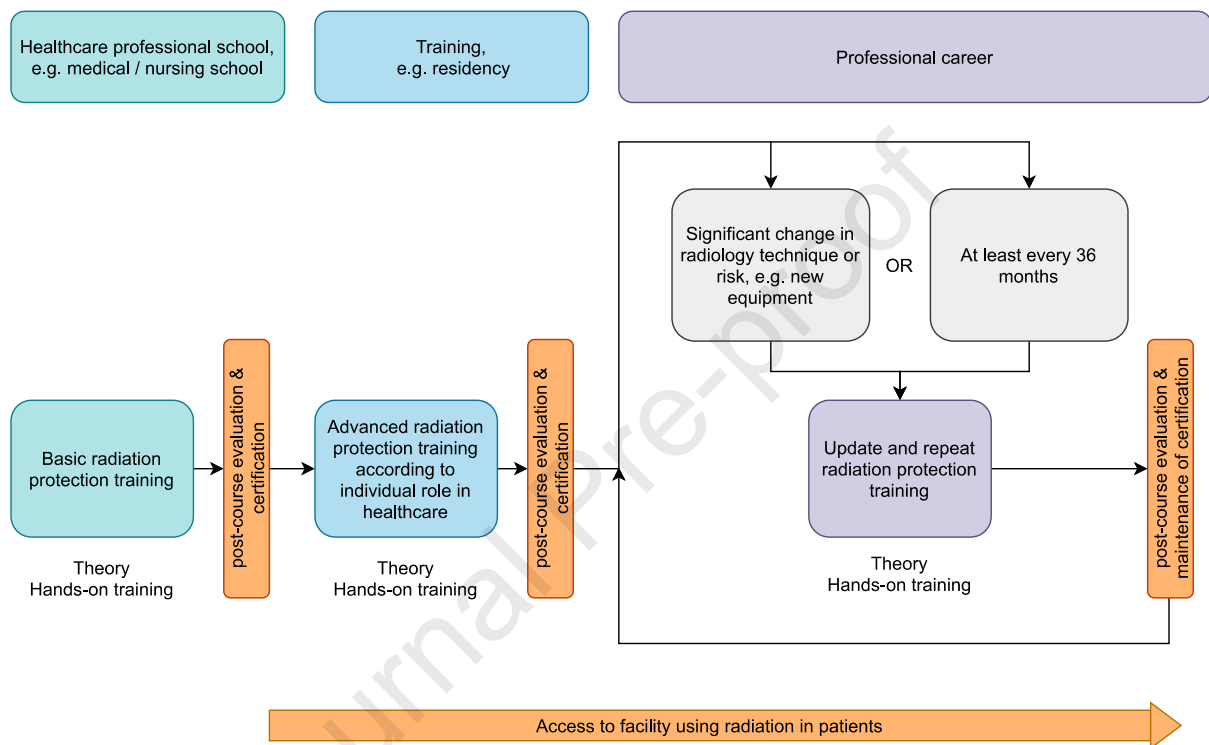

2173

2174

Chapter 8. Future technologies and gaps in evidence

Many of the recommendations outlined in these guidelines are supported by level C evidence and are reliant on the expert opinion of the committee. This highlights the need for the vascular community and allied disciplines to instigate studies that will strengthen the evidence base for radiation protection matters. New technologies that offer the promise of performing endovascular procedures with a reduced requirement for Xray guidance should be embraced and evaluated carefully according to standard innovation frameworks such as Idea, Development, Exploration, Assessment, Long term study (IDEAL). This chapter will outline developments currently taking place and future areas of research that may circumvent the limitations and dangers associated with Xray guidance for procedures.

8.1 New technologies

8.1.1 Three dimensional (3D) navigation


Images of guidewires, catheters and other endovascular devices are two dimensional (2D) and only available as grayscale images, which limits the ability to assess spatial relations between the devices and the vascular anatomy. It also limits the ability to identify the three dimensional (3D) shape and orientation of devices and significantly hinders navigation in the patient.

Recently, new technologies have been developed to enable 3D navigation of endovascular devices inside the body with a significant reduction in radiation dose. Two of these technologies include electromagnetic (EM) tracking and Fiber Optic RealShape Technology (FORS) and have shown potential in pre-clinical studies.³⁶⁹⁻³⁷²

An EM endovascular navigation system (ENS) provides the 3D position and orientation of EM coils (and thus the endovascular devices) and visualises the location of the coil in a pre-operative CT scan. This technology enables real time 3D imaging of endovascular devices, including stent graft positioning,³⁷³ in a radiation free environment. Pre-clinical reports are encouraging,^{370, 371} especially

when EM technology is used in combination with flexible robotic catheters, but clinical results are not as yet published.³⁷⁴

The Fiber Optic RealShape (FORS technology platform consists of equipment that sends laser light through a multicore optical fibre which is incorporated in endovascular guidewires and catheters. By analysing the reflected light it is possible to reconstruct the 3D shape of the full length of the optical fibre and thus of the endovascular devices (Figure 17).³⁷² An advantage of FORS compared with EM tracking is that FORS is able to show the endovascular devices over the entire length of the devices, whereas EM tracking technology only shows the tip of the devices, where the EM sensor is positioned. In a preclinical setting, safety and feasibility of the FORS system were demonstrated by the combined outcomes of high cannulation success, lack of hazards, positive user experience, and adequate accuracy.³⁷² FORS also allowed working in extreme views not achievable with standard gantry positions and also allows working simultaneously in two different angulations (e.g. AP and 90°). A first in human clinical feasibility study confirmed safety and feasibility of the FORS technology in endovascular procedures of the abdominal aorta and peripheral arteries and is now in use for catheterisation of target vessels during complex EVAR.^{375,376} Clinical studies with larger series of patients, however, are necessary to determine whether FORS has an effect on technical success rates, radiation parameters and procedural time in clinical practice.

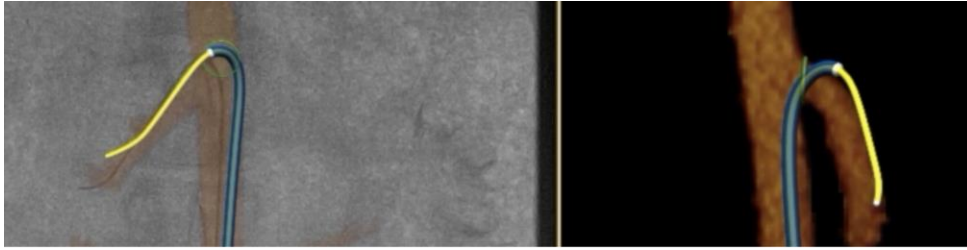

2217

2218 Figure 17: Endovascular procedure using FORS technology. Guidewire and catheter are shown in real
2219 time, in distinctive colours and with 3 Dimensional effects. The white dot on the devices shows the
2220 pointing direction of the tip.

2221

2222 8.1.2 Robotic tracking

2223 Robotic navigation systems may improve steerability of endovascular devices while allowing remote
2224 control and may be of particular benefit for complex EVAR cases, such as F/BEVAR. Robotic
2225 catheterisation of target vessels in a model simulating fenestrated stent grafting was carried out with
2226 negligible radiation exposure to the operator. Vessel cannulation times were reduced, with a
2227 significant reduction in the number of movements compared with conventional cannulation
2228 techniques.³⁷⁷

Previous clinical evaluation of a robotic navigation system has shown that it can be used safely for cannulation of renal and visceral target arteries during complex endovascular aortic procedures. It was found to be most effective for branched and chimney grafts, with an acceptable successful cannulation rate during fenestrated stent grafting (81%).³⁷⁸

Prospective studies are, however, needed to prove the clinical advantages of robotic navigation.

8.1.3 Artificial Intelligence

Introduction of AI technologies in fluoroscopy guided interventions may also reduce radiation doses. For example, the ability to use AI to make automatic adjustments to how guidewires and catheters appear on screen, may reduce the radiation exposure associated with tracking these devices to the desired anatomical location. AI algorithms can automatically recognise devices and trigger real time segmentations and improvements in visualisation, i.e., by showing the devices in distinctive colours and in higher resolution, allowing easier tracking and requiring less radiation exposure. Several groups are currently working on development of AI technologies for this indication.^{379, 380}

Another potential application of AI is automated recognition of the site of intervention within a fluoroscopy image. Radiation can then be delivered selectively to this region of interest (ROI). An integrated AI fluoroscopy (AIF) system has been used for Xray guided endoscopic procedures whereby a trained deep neural network recognises the ROI and subsequently performs ultrafast, automated collimation. In a prospective study of 100 patients, radiation exposure was compared in those who had endoscopic procedures using either a conventional or AI equipped fluoroscopy system. Radiation exposure to patients was significantly lower for the AIF system compared with the conventional fluoroscopy system, evidenced by a reduction in DAP from 5.7 mGym² to 2.2 mGym² (*p*

< .001) and almost 60% less radiation scatter.³⁸¹ Application of similar AIF systems for performing endovascular procedures would merit research.

Other desired AI driven technologies would include those that facilitate automated intra-operative dose reduction and also algorithms that drive warning systems, for example, those that trigger when operators fail to step back adequately during DSA acquisitions.

8.2 Gaps in practice and evidence

8.2.1 Global harmonisation of radiation safety practices

As discussed in chapter 2, the European legislation is clear in terms of dose limits and the high level needs for management of occupational, public and medical exposures. However, many of the details related to how to educate and manage the day to day practices in terms of personal protection equipment, dosimetry and monitoring are left to national regulations. Further, there is very little by way of international standardisation of regulatory practices. In order to promote global harmonisation, this standardisation needs to be established, through closer regional and national working.

An important consideration is low and middle income countries, where resources are limited. In these environments the most cost effective means of reducing radiation exposure should be identified and prioritised to allow the best protection that is feasible.

8.2.2 Radiation dose reference levels

Evaluation of the literature carried out for collation of these guidelines has shown a large variation in published radiation doses used for performing endovascular procedures. Two of the reasons for this variability are the endovascular operators' technique and the C arm equipment used. The expected radiation dose for a standard procedure should be better defined. This will come from standardised collection of procedure specific dose values for all endovascular operations. Two dosimetric

parameters that should be routinely collected and are offered by most Xray guidance equipment regardless of the hardware and manufacturer are Air-Kerma Area Product and Air Kerma at the patient entrance reference point (see chapter 2.2). Working groups can then use these data to set national DRLs (see chapter 2) for endovascular procedures and facilitate the use of radiation dosage as an additional quality metric for centres performing these procedures.

8.2.3 Pregnant staff in the endovascular operating room

As discussed in chapter 2, regulations clearly stipulate that unborn children of radiation workers are subject to the public dose limits, i.e., within the EU, 1 mGy per year.⁸ Some work has focused on how this is managed in practice in various different medical exposure settings, however, there is little by way of standardisation of practice in this area. Further work is urgently needed regarding how to best minimise risks and support safe normal working for pregnant staff in the endovascular operating environment. This should also include better education of personnel and employers with regard to the special considerations required for pregnant workers who are exposed to occupational radiation.

8.2.4 Biological correlates of radiation exposure

More radiobiological mechanistic and epidemiological research, and better linkage between these two areas, is needed to clearly determine the health effects of ionising radiation exposures. A key open question regards how risks vary with age, and this is especially important for younger patients who will live longer post-radiation exposure, and thus who have larger total risks of developing radiation induced cancers, for example. It is also important to increase knowledge regarding individual risks of radiation exposures, both for patients and for staff working with a variety of different exposure scenarios, with varying annual doses depending on a wide range of factors including training, use of dosimetry and personal protection equipment. Use of cutting edge

biological techniques, including genetic profiling may in the future identify individuals at particular risk from occupational radiation exposure and may even guide their career decisions.³⁸² Validation of microRNAs and non-coding RNAs in chronically exposed personnel may reveal novel biomarkers of exposure and sensitivity to exposure. Another area that requires attention is better prospective monitoring of health outcomes in radiation exposed medical staff. Without long term data collection on the incidence of cancer in these individuals, for example, we will never know if occupational radiation exposure truly increases the risk of malignancy in these individuals. The larger studies currently available are not conclusive as risks are low and the statistical power of these studies are not high enough. The advent of innovative study design and analysis for rare events may circumvent limitations encountered to date,

8.2.5 The value of real time dosimetry

It would seem intuitive that the use of real time dosimetry, providing a second by second readout of the effect of the operator's action on radiation exposure, would promote radiation safety. This has not been proven conclusively, however, and more studies are needed to objectively determine the additional role of this adjunct in relation to the other safety behaviours adopted in the endovascular operating room. Specifically, observational studies that aim to quantify the radiation dose savings in operators wearing real time dosimeters and any behaviour modifications that result from the operator watching their dose rise. Such studies would also allow operator doses to be related to doses absorbed by the patient. Expected benefits of real time dosimetry with direct feedback need to be confirmed and quantified for endovascular procedures in clinical comparative series.

8.2.6 Operator control of C arm equipment

In most countries, trained endovascular operator control of the C arm is preferred to assistant control. It is perceived that this will reduce radiation exposure since the operator knows precisely when to initiate and cease screening based upon the intended purpose. Furthermore, the operator

can specifically set the appropriate acquisition parameters such as collimation, magnification and frame rate, thereby limiting exposure and scatter and focusing upon the region of interest involved in that specific part of the procedure. There is, however, limited evidence to support this notion and further studies are needed that quantify radiation exposure according to workflow within the endovascular operating room, including the individuals who are responsible for controlling the C arm.

8.2.7 Personal protection equipment

The additional value of leg shields needs to be defined. Available evidence is so far limited to a single study and further data are needed, especially in combination with other protection devices.

The additional value of full body shields needs to be supported by clinical data. Also, the high cost of the only system available today also means that cost aspects need to be highlighted. Alternative whole body protection needs to be developed and evaluated.

Reports of potential lead contamination on lead aprons are worrying, and the extent and significance of this need to be clarified urgently.

8.2.8 Education and training

Radiation protection training is mostly regulated by national authorities. Ideally these regulations should be reviewed and compared across the European member states to study any similarities and differences, allowing authorities to optimise or adjust their regulations about radiation protection training.

It is important that structured programmes are established for training the trainers in radiation safety. An ideal model might be for an appropriately trained medical physicist and a healthcare professional who uses radiation in day to day work in the endovascular operating room to run

2348 radiation safety courses together. In addition, the impact of radiation safety courses on the
2349 knowledge, skills and behaviour of trainees who attend should be studied in a more structured way
2350 to objectively assess benefits.

2351 Augmented reality and VR simulation is likely to play an increasingly prominent role in preparing
2352 healthcare personnel prior to working in the endovascular operating room. Practice in environments
2353 created using these technologies may help raise awareness about factors associated with radiation
2354 exposure of endovascular team members and aid personnel in: (i) putting into practice radiation
2355 safety knowledge they have gained; (ii) learning how to use modern technologies safely; and (iii) to
2356 improve the radiation safety behaviour in endovascular practice to protect both endovascular
2357 operator and patient. Multicentre trials are needed to demonstrate any benefit related to these
2358 modern educational materials in order to justify the investment made.

2359 The impact of radiation safety training (knowledge, skills and behaviour) on behaviours of the team
2360 members in the endovascular operating room should be evaluated regularly. This can be done by
2361 combining reliable rating scale evaluations, real time dosimeters, dose registration software,
2362 structured dose reports and possibly artificial intelligence technologies. This may provide detailed
2363 information about key aspects of the entire endovascular team's radiation safety behaviour, facilitate
2364 targeted feedback and the development of radiation safety training interventions. This allows a
2365 targeted approach adapted to the needs of that particular team.

REFERENCES

1. Schanzer A, Steppacher R, Eslami M, Arous E, Messina L, Belkin M. Vascular surgery training trends from 2001-2007: A substantial increase in total procedure volume is driven by escalating endovascular procedure volume and stable open procedure volume. *J Vasc Surg.* 2009;49:1339-44.
2. Beck AW, Sedrakyan A, Mao J, Venermo M, Faizer R, Debus S, et al. Variations in Abdominal Aortic Aneurysm Care: A Report From the International Consortium of Vascular Registries. *Circulation.* 2016;134:1948-58.
3. Suckow BD, Goodney PP, Columbo JA, Kang R, Stone DH, Sedrakyan A, et al. National trends in open surgical, endovascular, and branched-fenestrated endovascular aortic aneurysm repair in Medicare patients. *J Vasc Surg.* 2018;67:1690-7 e1.
4. Behrendt CA, Sigvant B, Kuchenbecker J, Grima MJ, Schermerhorn M, Thomson IA, et al. Editor's Choice - International Variations and Sex Disparities in the Treatment of Peripheral Arterial Occlusive Disease: A Report from VASCUNET and the International Consortium of Vascular Registries. *Eur J Vasc Endovasc Surg.* 2020;60:873-80.
5. Kirkwood ML, Guild JB, Arbique GM, Anderson JA, Valentine RJ, Timaran C. Surgeon radiation dose during complex endovascular procedures. *J Vasc Surg.* 2015;62:457-63.
6. El-Sayed T, Patel AS, Cho JS, Kelly JA, Ludwinski FE, Saha P, et al. Radiation-Induced DNA Damage in Operators Performing Endovascular Aortic Repair. *Circulation.* 2017;136:2406-16.
7. Mohapatra A, Greenberg RK, Mastracci TM, Eagleton MJ, Thornsberry B. Radiation exposure to operating room personnel and patients during endovascular procedures. *J Vasc Surg.* 2013;58:702-9.

- 2388 8. Council Directive 2013/59/EURATOM of 5 December 2013 laying down basic safety standards
2389 for protection against the dangers arising from exposure to ionising radiation, and repealing
2390 Directives 89/618/Euratom, 90/641/Euratom, 96/29/Euratom, 97/43/Euratom and
2391 2003/122/Euratom. Official Journal of the European Union [https://eur-lex.europa.eu/legal-](https://eur-lex.europa.eu/legal-content/EN/TXT/?qid=1561896809548&uri=CELEX:32013L0059)
2392 [content/EN/TXT/?qid=1561896809548&uri=CELEX:32013L0059](https://eur-lex.europa.eu/legal-content/EN/TXT/?qid=1561896809548&uri=CELEX:32013L0059).
- 2393 9. ICRP. Occupational radiological protection in interventional procedures. ICRP Publication 139.
2394 Ann ICRP. 2018;47.
- 2395 10. ICRP. Radiological Protection in Fluoroscopically Guided Procedures outside the Imaging
2396 Department. ICRP Publication 117. Ann ICRP. 2010;40.
- 2397 11. ICRP. Avoidance of Radiation Injuries from Medical Interventional Procedures. ICRP
2398 Publication 85. Ann ICRP. 2000;30.
- 2399 12. Fletcher DW, Miller DL, Balter S, Taylor MA. Comparison of four techniques to estimate
2400 radiation dose to skin during angiographic and interventional radiology procedures. J Vasc Interv
2401 Radiol. 2002;13:391-7.
- 2402 13. Miller DL, Balter S, Cole PE, Lu HT, Schueler BA, Geisinger M, et al. Radiation doses in
2403 interventional radiology procedures: the RAD-IR study: part I: overall measures of dose. J Vasc Interv
2404 Radiol. 2003;14:711-27.
- 2405 14. Miller DL, Balter S, Wagner LK, Cardella J, Clark TW, Neithamer CDJ, et al. Quality
2406 improvement guidelines for recording patient radiation dose in the medical record. J Vasc Interv
2407 Radiol. 2004;15:423-9.
- 2408 15. National Council on Radiation Protection and Measurements. Radiation dose management
2409 for fluoroscopically-guided interventional medical procedures. NCRP Report No. 168. 2010.

- 2410 16. Chait J, Davis N, Ostrozhynskyy Y, Rajae S, Marks N, Hingorani A, et al. Radiation exposure
2411 during non-thrombotic iliac vein stenting. *Vascular*. 2019;27:617-22.
- 2412 17. Barbati ME, Gombert A, Schleimer K, Kotelis D, Wittens CHA, Bruners P, et al. Assessing
2413 radiation exposure to patients during endovascular treatment of chronic venous obstruction. *J Vasc*
2414 *Surg Venous Lymphat Disord*. 2019;7:392-8.
- 2415 18. Lim CS, Waseem S, El-Sayed T, Budge J, Quintana B, Thulasidasan N, et al. Patient radiation
2416 exposure for endovascular deep venous interventions. *J Vasc Surg Venous Lymphat Disord*.
2417 2020;8:259-67.
- 2418 19. Baccellieri D, Apruzzi L, Ardita V, Bilman V, De Cobelli F, Melissano G, et al. Intraoperative
2419 completion cone-beam computed tomography for the assessment of residual lesions after primary
2420 treatment of proximal venous outflow obstructions. *Phlebology*. 2022;37:55-62.
- 2421 20. Tuthill E, O'Hora L, O'Donohoe M, Panci S, Gilligan P, Campion D, et al. Investigation of
2422 reference levels and radiation dose associated with abdominal EVAR (endovascular aneurysm repair)
2423 procedures across several European Centres. *Eur Radiol*. 2017;27:4846-56.
- 2424 21. Farah J, Gonzalez-Mendez LA, Dufay F, Amir S, Royer B, Gabriel H, et al. Patient exposure and
2425 diagnostic reference levels in operating rooms: a multi-centric retrospective study in over 150 private
2426 and public French clinics. *J Radiol Prot*. 2020.
- 2427 22. Vassileva J, Rehani M. Diagnostic reference levels. *AJR Am J Roentgenol*. 2015;204:W1-3.
- 2428 23. ICRP. Diagnostic reference levels in medical imaging. ICRP Publication 135. *Ann ICRP*.
2429 2017;46.
- 2430 24. Rial R, Vañó E, Río-Solá MLD, Fernández JM, Sánchez RM, Santervás LAC, et al. National
2431 Diagnostic Reference Levels for Endovascular Aneurysm Repair and Optimisation Strategies. *Eur J*
2432 *Vasc Endovasc Surg*. 2020;60:837-42.

- 2433 25. Koenig TR, Wolff D, Mettler FA, K. WL. Skin injuries from fluoroscopically guided procedures:
2434 part 1, characteristics of radiation injury. AJR Am J Roentgenol. 2001;177:3-11.
- 2435 26. Koenig TR, Mettler FA, Wagner LK. Skin Injuries from Fluoroscopically Guided Procedures:
2436 Part 2, Review of 73 Cases and Recommendations for Minimizing Dose Delivered to Patient. AJR Am J
2437 Roentgenol. 2001;177:13-20.
- 2438 27. DiCarlo AL, Bandremer AC, Hollingsworth BA, Kasim S, Laniyonu A, Todd NF, et al. Cutaneous
2439 Radiation Injuries: Models, Assessment and Treatments. Radiat Res. 2020;194:315-44.
- 2440 28. ICRP. ICRP Statement on Tissue Reactions / Early and Late Effects of Radiation in Normal
2441 Tissues and Organs – Threshold Doses for Tissue Reactions in a Radiation Protection Context. ICRP
2442 Publication 118. Ann ICRP. 2012;41.
- 2443 29. Ozasa K, Grant EJ, Kodama K. Japanese Legacy Cohorts: The Life Span Study Atomic Bomb
2444 Survivor Cohort and Survivors' Offspring. J Epidemiol. 2018;28:162-9.
- 2445 30. National Research Council. Health Risks from Exposure to Low Levels of Ionizing Radiation:
2446 BEIR VII Phase 2. Washington, DC: The National Academies Press; 2006. 422 p.
- 2447 31. Calabrese EJ. Hormesis: Path and Progression to Significance. Int J Mol Sci. 2018;19.
- 2448 32. Boice JD. The linear nonthreshold (LNT) model as used in radiation protection: an NCRP
2449 update. Int J Radiat Biol. 2017;93:1079-92.
- 2450 33. ICRP. The 2007 Recommendations of the International Commission on Radiological
2451 Protection. ICRP Publication 103. Ann ICRP. 2007;36:2-4.
- 2452 34. Tapiovaara M, Siiskonen T. PCXMC: A Monte Carlo program for calculating patient doses in
2453 medical x-ray examinations. STUK - Radiation and Nuclear Safety Authority, Editor. Helsinki, Finland,
2454 2008.

- 2455 35. Borrego D, Lowe EM, Kitahara CM, Lee C. Assessment of PCXMC for patients with different
2456 body size in chest and abdominal x ray examinations: a Monte Carlo simulation study. *Phys Med Biol*.
2457 2018;63:065015.
- 2458 36. Harbron RW, Abdelhalim M, Ainsbury EA, Eakins JS, Alam A, Lee C, et al. Patient radiation
2459 dose from x-ray guided endovascular aneurysm repair: a Monte Carlo approach using voxel
2460 phantoms and detailed exposure information. *J Radiol Prot*. 2020;40:704-26.
- 2461 37. Mathews JD, Forsythe AV, Brady Z, Butler MW, Goergen SK, Byrnes GB, et al. Cancer risk in
2462 680,000 people exposed to computed tomography scans in childhood or adolescence: data linkage
2463 study of 11 million Australians. *BMJ*. 2013;346:f2360.
- 2464 38. Vano E, Gonzalez L, Fernandez JM, Guibelalde E. Patient dose values in interventional
2465 radiology. *Br J Radiol*. 1995;68:1215-20.
- 2466 39. Sanchez R, Vano E, Fernandez JM, Machado A, Roas N. Visual and numerical methods to
2467 measure patient skin doses in interventional procedures using radiochromic XR-RV2 films. *Radiat*
2468 *Prot Dosimetry*. 2011;147:94-8.
- 2469 40. Ding GX, Malcolm AW. An optically stimulated luminescence dosimeter for measuring patient
2470 exposure from imaging guidance procedures. *Phys Med Biol*. 2013;58:5885-97.
- 2471 41. Struelens L, Bacher K, Bosmans H, Bleeser F, Hoornaert MT, Malchair F, et al. Establishment
2472 of trigger levels to steer the follow-up of radiation effects in patients undergoing fluoroscopically-
2473 guided interventional procedures in Belgium. *Phys Med*. 2014;30:934-40.
- 2474 42. den Boer A, de Feijter PJ, Serruys PW, Roelandt JR. Real-time quantification and display of
2475 skin radiation during coronary angiography and intervention. *Circulation*. 2001;104:1779-84.

- 2476 43. Khodadadegan Y, Zhang M, Pavlicek W, Paden RG, Chong B, Schueler BA, et al. Automatic
 2477 monitoring of localized skin dose with fluoroscopic and interventional procedures. J Digit Imaging.
 2478 2011;24:626-39.
- 2479 44. Rana VK, Rudin S, Bednarek DR. A tracking system to calculate patient skin dose in real-time
 2480 during neurointerventional procedures using a biplane x-ray imaging system. Med Phys.
 2481 2016;43:5131.
- 2482 45. Sanchez RM, Vano E, Fernandez JM, Escaned J. Evaluation of a real-time display for skin dose
 2483 map in cardiac catheterisation procedures. Radiat Prot Dosimetry. 2015;165:240-3.
- 2484 46. Sanchez RM, Vano E, Fernandez JM, Ten JJ, Mendez Montero JV, Armijo J et al. Experience
 2485 with a real time patient skin dose distribution estimator for interventional radiology. European
 2486 Congress of Radiology 2017 poster.
- 2487 47. Stecker MS, Balter S, Towbin RB, Miller DL, Vañó E, Bartal G, et al. Guidelines for patient
 2488 radiation dose management. J Vasc Interv Radiol. 2009;20:S263-73.
- 2489 48. Lee WH, Nguyen PK, Fleischmann D, Wu JC. DNA damage-associated biomarkers in studying
 2490 individual sensitivity to low-dose radiation from cardiovascular imaging. Eur Heart J. 2016;37:3075-
 2491 80.
- 2492 49. Beels L, Bacher K, De Wolf D, Werbrouck J, Thierens H. gamma-H2AX foci as a biomarker for
 2493 patient X-ray exposure in pediatric cardiac catheterization: are we underestimating radiation risks?
 2494 Circulation. 2009;120:1903-9.
- 2495 50. Sari-Minodier I, Orsière T, Auquier P, Martin F, Botta A. Cytogenetic monitoring by use of the
 2496 micronucleus assay among hospital workers exposed to low doses of ionizing radiation. Mutat Res.
 2497 2007;629:111-21.

- 2498 51. Zakeri F, Hirobe T. A cytogenetic approach to the effects of low levels of ionizing radiations
2499 on occupationally exposed individuals. *Eur J Radiol.* 2010;73:191-5.
- 2500 52. Nguyen PK, Lee WH, Li YF, Hong WX, Hu S, Chan C, et al. Assessment of the Radiation Effects
2501 of Cardiac CT Angiography Using Protein and Genetic Biomarkers. *JACC Cardiovasc Imaging.*
2502 2015;8:873-84.
- 2503 53. Borghini A, Vecoli C, Mercuri A, Carpeggiani C, Piccaluga E, Guagliumi G, et al. Low-Dose
2504 Exposure to Ionizing Radiation Deregulates the Brain-Specific MicroRNA-134 in Interventional
2505 Cardiologists. *Circulation.* 2017;136:2516-8.
- 2506 54. Hall J, Jeggo PA, West C, Gomolka M, Quintens R, Badie C, et al. Ionizing radiation biomarkers
2507 in epidemiological studies - An update. *Mutat Res Rev Mutat Res.* 2017;771:59-84.
- 2508 55. Patel R, Sweeting MJ, Powell JT, Greenhalgh RM, investigators Et. Endovascular versus open
2509 repair of abdominal aortic aneurysm in 15-years' follow-up of the UK endovascular aneurysm repair
2510 trial 1 (EVAR trial 1): a randomised controlled trial. *Lancet.* 2016;388:2366-74.
- 2511 56. Markar SR, Vidal-Diez A, Sounderajah V, Mackenzie H, Hanna GB, Thompson M, et al. A
2512 population-based cohort study examining the risk of abdominal cancer after endovascular abdominal
2513 aortic aneurysm repair. *J Vasc Surg.* 2019;69:1776-85.e2.
- 2514 57. Zoli S, Trabattoni P, Dainese L, Annoni A, Saccu C, Fumagalli M, et al. Cumulative radiation
2515 exposure during thoracic endovascular aneurysm repair and subsequent follow-up. *Eur J*
2516 *Cardiothorac Surg.* 2012;42:254-9; discussion 9-60.
- 2517 58. Balter S, Hopewell JW, Miller DL, Wagner LK, Zelefsky MJ. Fluoroscopically guided
2518 interventional procedures: a review of radiation effects on patients' skin and hair. *Radiology.*
2519 2010;254:326-41.

- 2520 59. Weerakkody RA, Walsh SR, Cousins C, Goldstone KE, Tang TY, Gaunt ME. Radiation exposure
2521 during endovascular aneurysm repair. *Br J Surg.* 2008;95:699-702.
- 2522 60. Kirkwood ML, Arbique GM, Guild JB, Timaran C, Anderson JA, Valentine RJ. Deterministic
2523 effects after fenestrated endovascular aortic aneurysm repair. *J Vasc Surg.* 2015;61:902-6.
- 2524 61. Kirkwood ML, Arbique GM, Guild JB, Timaran C, Valentine RJ, Anderson JA. Radiation-induced
2525 skin injury after complex endovascular procedures. *J Vasc Surg.* 2014;60:742-8.
- 2526 62. Walsh SR, Cousins C, Tang TY, Gaunt ME, Boyle JR. Ionizing Radiation in Endovascular
2527 Interventions. *J Endovasc Ther.* 2008;15:680-7.
- 2528 63. Zielinski JM, Garner MJ, Band PR, Krewski D, Shilnikova NS, Jiang H, et al. Health outcomes of
2529 low-dose ionizing radiation exposure among medical workers: a cohort study of the Canadian
2530 national dose registry of radiation workers. *Int J Occup Med Environ Health.* 2009;22:149-56.
- 2531 64. Preston DL, Kitahara CM, Freedman DM, Sigurdson AJ, Simon SL, Little MP, et al. Breast
2532 cancer risk and protracted low-to-moderate dose occupational radiation exposure in the US
2533 Radiologic Technologists Cohort, 1983-2008. *Br J Cancer.* 2016;115:1105-12.
- 2534 65. Rajaraman P, Doody MM, Yu CL, Preston DL, Miller JS, Sigurdson AJ, et al. Cancer Risks in U.S.
2535 Radiologic Technologists Working With Fluoroscopically Guided Interventional Procedures, 1994-
2536 2008. *AJR Am J Roentgenol.* 2016;206:1101-8.
- 2537 66. Yoshinaga S, Hauptmann M, Sigurdson AJ, Doody MM, Freedman DM, Alexander BH, et al.
2538 Nonmelanoma skin cancer in relation to ionizing radiation exposure among U.S. radiologic
2539 technologists. *Int J Cancer.* 2005;115:828-34.
- 2540 67. Leuraud K, Richardson DB, Cardis E, Daniels RD, Gillies M, O'Hagan JA, et al. Ionising radiation
2541 and risk of death from leukaemia and lymphoma in radiation-monitored workers (INWORKS): an
2542 international cohort study. *Lancet Haematol.* 2015;2:e276-81.

- 2543 68. Andreassi MG, Piccaluga E, Guagliumi G, Del Greco M, Gaita F, Picano E. Occupational Health
2544 Risks in Cardiac Catheterization Laboratory Workers. *Circ Cardiovasc Interv.* 2016;9:e003273.
- 2545 69. Wang JX, Zhang LA, Li BX, Zhao YC, Wang ZQ, Zhang JY, et al. Cancer incidence and risk
2546 estimation among medical x-ray workers in China, 1950-1995. *Health Phys.* 2002;82:455-66.
- 2547 70. Berrington A, Darby SC, Weiss HA, Doll R. 100 years of observation on British radiologists:
2548 mortality from cancer and other causes 1897-1997. *Br J Radiol.* 2001;74:507-19.
- 2549 71. Reeves RR, Ang L, Bahadorani J, Naghi J, Dominguez A, Palakodeti V, et al. Invasive
2550 Cardiologists Are Exposed to Greater Left Sided Cranial Radiation: The BRAIN Study (Brain Radiation
2551 Exposure and Attenuation During Invasive Cardiology Procedures). *JACC Cardiovasc Interv.*
2552 2015;8:1197-206.
- 2553 72. Roguin A, Goldstein J, Bar O, Goldstein JA. Brain and neck tumors among physicians
2554 performing interventional procedures. *Am J Cardiol.* 2013;111:1368-72.
- 2555 73. Kitahara CM, Linet MS, Balter S, Miller DL, Rajaraman P, Cahoon EK, et al. Occupational
2556 Radiation Exposure and Deaths From Malignant Intracranial Neoplasms of the Brain and CNS in U.S.
2557 Radiologic Technologists, 1983-2012. *AJR Am J Roentgenol.* 2017;208:1278-84.
- 2558 74. Kleiman NJ. Radiation cataract. *Ann ICRP.* 2012;41:80-97.
- 2559 75. Klein LW, Miller DL, Balter S, Laskey W, Haines D, Norbash A, et al. Occupational health
2560 hazards in the interventional laboratory: time for a safer environment. *Radiology.* 2009;250:538-44.
- 2561 76. Worgul BV, Kundiyeve YI, Sergiyenko NM, Chumak VV, Vitte PM, Medvedovsky C, et al.
2562 Cataracts among Chernobyl clean-up workers: implications regarding permissible eye exposures.
2563 *Radiat Res.* 2007;167:233-43.

- 2564 77. Jungi S, Ante M, Geisbusch P, Hoedlmoser H, Kleinau P, Bockler D. Protected and
2565 Unprotected Radiation Exposure to the Eye Lens during Endovascular Procedures in Hybrid Operating
2566 Rooms. *Eur J Vasc Endovasc Surg*. 2022.
- 2567 78. Chodick G, Bekiroglu N, Hauptmann M, Alexander BH, Freedman DM, Doody MM, et al. Risk
2568 of cataract after exposure to low doses of ionizing radiation: a 20-year prospective cohort study
2569 among US radiologic technologists. *Am J Epidemiol*. 2008;168:620-31.
- 2570 79. Elmaraezy A, Ebraheem Morra M, Tarek Mohammed A, Al-Habaa A, Elgebaly A,
2571 Abdelmotaleb Ghazy A, et al. Risk of cataract among interventional cardiologists and catheterization
2572 lab staff: A systematic review and meta-analysis. *Catheter Cardiovasc Interv*. 2017;90:1-9.
- 2573 80. Karatasakis A, Brilakis HS, Danek BA, Karacsonyi J, Martinez-Parachini JR, Nguyen-Trong PJ, et
2574 al. Radiation-associated lens changes in the cardiac catheterization laboratory: Results from the IC-
2575 CATARACT (CATaracts Attributed to RAdiation in the CaTh lab) study. *Catheter Cardiovasc Interv*.
2576 2018;91:647-54.
- 2577 81. Bhatti P, Sigurdson AJ, Mabuchi K. Can low-dose radiation increase risk of cardiovascular
2578 disease? *Lancet*. 2008;372:697-9.
- 2579 82. Little MP, Tawn EJ, Tzoulaki I, Wakeford R, Hildebrandt G, Paris F, et al. A systematic review
2580 of epidemiological associations between low and moderate doses of ionizing radiation and late
2581 cardiovascular effects, and their possible mechanisms. *Radiat Res*. 2008;169:99-109.
- 2582 83. Galper SL, Yu JB, Mauch PM, Strasser JF, Silver B, Lacasce A, et al. Clinically significant cardiac
2583 disease in patients with Hodgkin lymphoma treated with mediastinal irradiation. *Blood*.
2584 2011;117:412-8.
- 2585 84. Taylor CW, McGale P, Darby SC. Cardiac risks of breast-cancer radiotherapy: a contemporary
2586 view. *Clin Oncol (R Coll Radiol)*. 2006;18:236-46.

- 2587 85. Liu JJ, Freedman DM, Little MP, Doody MM, Alexander BH, Kitahara CM, et al. Work history
2588 and mortality risks in 90,268 US radiological technologists. *Occup Environ Med.* 2014;71:819-35.
- 2589 86. European Commission Directorate-General for Energy Directorate D — Nuclear Safety & Fuel
2590 Cycle Unit D.3 — Radiation Protection. European Guidelines on Medical Physics Expert. Radiation
2591 Protection No. 174. 2014. <https://ec.europa.eu/energy/sites/ener/files/documents/174.pdf>.
2592 Accessed 9 January, 2020.
- 2593 87. Casar B, Lopes Mdo C, Drljevic A, Gershkevitch E, Pesznyak C. Medical physics in Europe
2594 following recommendations of the International Atomic Energy Agency. *Radiol Oncol.* 2016;50:64-72.
- 2595 88. National Council on Radiation Protection and Measurements. Medical Radiation Exposure of
2596 Patients in the United States. NCRP Report No. 184. 2019.
- 2597 89. Mettler FA, Jr., Mahesh M, Bhargavan-Chatfield M, Chambers CE, Elee JG, Frush DP, et al.
2598 Patient Exposure from Radiologic and Nuclear Medicine Procedures in the United States: Procedure
2599 Volume and Effective Dose for the Period 2006-2016. *Radiology.* 2020;295:418-27.
- 2600 90. National Council on Radiation Protection and Measurements. Preconception and Prenatal
2601 Radiation Exposure: Health Effects and Protective Guidance. NCRP Report No. 174. 2013.
- 2602 91. Oatway W, Jones A, Holmes S, Watson S, Cabianca T. Ionising Radiation Exposure of the UK
2603 Population: 2010 Review. PHE Report Series PHE-CRCE-026. 2016. [https://www.phe-](https://www.phe-protection-services.org.uk/cms/assets/gfx/content/resource_3595csc0e8517b1f.pdf)
2604 [protection-services.org.uk/cms/assets/gfx/content/resource_3595csc0e8517b1f.pdf](https://www.phe-protection-services.org.uk/cms/assets/gfx/content/resource_3595csc0e8517b1f.pdf) (Accessed 20
2605 November 2020).
- 2606 92. Stahl CM, Meisinger QC, Andre MP, Kinney TB, Newton IG. Radiation Risk to the Fluoroscopy
2607 Operator and Staff. *AJR Am J Roentgenol.* 2016;207:737-44.
- 2608 93. Weiss S, Van Herzeele I. Radiation Protection Training for Vascular Surgeons in Twenty-One
2609 European Countries. *Eur J Vasc Endovasc Surg.* 2020;59:512-3.

- 2610 94. Shaw PM, Vouyouka A, Reed A. Time for radiation safety program guidelines for pregnant
2611 trainees and vascular surgeons. *J Vasc Surg.* 2012;55:862-8 e2.
- 2612 95. Bordoli SJ, Carsten CG, 3rd, Cull DL, Johnson BL, Taylor SM. Radiation safety education in
2613 vascular surgery training. *J Vasc Surg.* 2014;59:860-4.
- 2614 96. Kamiya K, Ozasa K, Akiba S, Niwa O, Kodama K, Takamura N, et al. Long-term effects of
2615 radiation exposure on health. *Lancet.* 2015;386:469-78.
- 2616 97. Grant EJ, Furukawa K, Sakata R, Sugiyama H, Sadakane A, Takahashi I, et al. Risk of death
2617 among children of atomic bomb survivors after 62 years of follow-up: a cohort study. *Lancet Oncol.*
2618 2015;16:1316-23.
- 2619 98. Dockerty J, Jolly J, Kumar A, Larsen T, McBride D, McGill S, et al. The New Zealand nuclear
2620 veteran and families study, exploring the options to assess heritable health outcomes. *N Z Med J.*
2621 2020;133:70-8.
- 2622 99. Vu CT, Elder DH. Pregnancy and the working interventional radiologist. *Semin Intervent*
2623 *Radiol.* 2013;30:403-7.
- 2624 100. Chandra V, Dorsey C, Reed AB, Shaw P, Banghart D, Zhou W. Monitoring of fetal radiation
2625 exposure during pregnancy. *J Vasc Surg.* 2013;58:710-4.
- 2626 101. Dauer LT, Thornton RH, Miller DL, Damilakis J, Dixon RG, Marx MV, et al. Radiation
2627 management for interventions using fluoroscopic or computed tomographic guidance during
2628 pregnancy: a joint guideline of the Society of Interventional Radiology and the Cardiovascular and
2629 Interventional Radiological Society of Europe with Endorsement by the Canadian Interventional
2630 Radiology Association. *J Vasc Interv Radiol.* 2012;23:19-32.
- 2631 102. Suarez RC, Berard P, Harrison JD, Melo DR, Nosske D, Stabin M, et al. Review of standards of
2632 protection for pregnant workers and their offspring. *Radiat Prot Dosimetry.* 2007;127:19-22.

- 2633 103. Chu B, Miodownik D, Williamson MJ, Gao Y, St Germain J, Dauer LT. Radiological protection
2634 for pregnant women at a large academic medical Cancer Center. *Phys Med*. 2017;43:186-9.
- 2635 104. Dauer LT, Miller DL, Schueler B, Silberzweig J, Balter S, Bartal G, et al. Occupational radiation
2636 protection of pregnant or potentially pregnant workers in IR: a joint guideline of the Society of
2637 Interventional Radiology and the Cardiovascular and Interventional Radiological Society of Europe. *J*
2638 *Vasc Interv Radiol*. 2015;26:171-81.
- 2639 105. Sarkozy A, De Potter T, Heidbuchel H, Ernst S, Kosiuk J, Vano E, et al. Occupational radiation
2640 exposure in the electrophysiology laboratory with a focus on personnel with reproductive potential
2641 and during pregnancy: A European Heart Rhythm Association (EHRA) consensus document endorsed
2642 by the Heart Rhythm Society (HRS). *Europace*. 2017;19:1909-22.
- 2643 106. Delichas M, Psarrakos K, Molyvda-Athanassopoulou E, Giannoglou G, Sioundas A,
2644 Hatzioannou K, et al. Radiation exposure to cardiologists performing interventional cardiology
2645 procedures. *Eur J Radiol*. 2003;48:268-73.
- 2646 107. Bartal G, Roguin A, Paulo G. Call for Implementing a Radiation Protection Culture in
2647 Fluoroscopically Guided Interventional Procedures. *AJR Am J Roentgenol*. 2016;206:1110-1.
- 2648 108. Attigah N, Oikonomou K, Hinz U, Knoch T, Demirel S, Verhoeven E, et al. Radiation exposure
2649 to eye lens and operator hands during endovascular procedures in hybrid operating rooms. *J Vasc*
2650 *Surg*. 2016;63:198-203.
- 2651 109. Chodick G, Bekiroglu N, Hauptmann M, Alexander BH, Freedman DM, Doody MM, et al. Risk
2652 of cataract after exposure to low doses of ionizing radiation: a 20-year prospective cohort study
2653 among US radiologic technologists. *Am J Epidemiol*. 2008;168:620-31.
- 2654 110. Vano E, Kleiman NJ, Duran A, Romano-Miller M, Rehani MM. Radiation-associated lens
2655 opacities in catheterization personnel: results of a survey and direct assessments. *J Vasc Interv*
2656 *Radiol*. 2013;24:197-204.

- 2657 111. Monastiriotis S, Comito M, Labropoulos N. Radiation exposure in endovascular repair of
2658 abdominal and thoracic aortic aneurysms. *J Vasc Surg.* 2015;62:753-61.
- 2659 112. Panuccio G, Greenberg RK, Wunderle K, Mastracci TM, Eagleton MG, Davros W. Comparison
2660 of indirect radiation dose estimates with directly measured radiation dose for patients and operators
2661 during complex endovascular procedures. *J Vasc Surg.* 2011;53:885-94 e1.
- 2662 113. Arai T, Uchino S, Kubo Y, Kiyama S, Uezono S. Radiation exposure to anaesthetists during
2663 endovascular procedures. *Anaesthesia.* 2015;70:47-50.
- 2664 114. Bacchim Neto FA, Alves AF, Mascarenhas YM, Nicolucci P, Pina DR. Occupational radiation
2665 exposure in vascular interventional radiology: A complete evaluation of different body regions. *Phys*
2666 *Med.* 2016;32:1019-24.
- 2667 115. National Council on Radiation Protection and Measurements. Use of personal monitors to
2668 estimate effective dose equivalent and effective dose to workers for external exposure to low-LET
2669 radiation. NCRP Report No. 122. 1995.
- 2670 116. Bordy JM, Gualdrini G, Daures J, Mariotti F. Principles for the design and calibration of
2671 radiation protection dosimeters for operational and protection quantities for eye lens dosimetry.
2672 *Radiat Prot Dosimetry.* 2011;144:257-61.
- 2673 117. Carinou E, Ferrari P, Bjelac OC, Gingaume M, Merce MS, O'Connor U. Eye lens monitoring for
2674 interventional radiology personnel: dosimeters, calibration and practical aspects of H p (3)
2675 monitoring. A 2015 review. *J Radiol Prot.* 2015;35:R17-34.
- 2676 118. Andrade G, Khoury HJ, Garzon WJ, Dubourcq F, Bredow MF, Monsignore LM, et al. Radiation
2677 Exposure of Patients and Interventional Radiologists during Prostatic Artery Embolization: A
2678 Prospective Single-Operator Study. *J Vasc Interv Radiol.* 2017;28:517-21.

- 2679 119. Anderson NE, King SH, Miller KL. Variations in dose to the extremities of
2680 vascular/interventional radiologists. *Health Phys.* 1999;76:S39-40.
- 2681 120. Albayati MA, Kelly S, Gallagher D, Dourado R, Patel AS, Saha P, et al. Editor's choice--
2682 Angulation of the C-arm during complex endovascular aortic procedures increases radiation exposure
2683 to the head. *Eur J Vasc Endovasc Surg.* 2015;49:396-402.
- 2684 121. European Commission Directorate-General for Energy and Transport Directorate H —
2685 Nuclear Energy Unit H.4 — Radiation Protection. Technical Recommendations for Monitoring
2686 Individuals Occupationally Exposed to External Radiation. Radiation Protection No. 160. 2009.
2687 <https://ec.europa.eu/energy/sites/ener/files/documents/160.pdf>.
- 2688 122. Miller DL, Balter S, Cole PE, Lu HT, Berenstein A, Albert R, et al. Radiation doses in
2689 interventional radiology procedures: the RAD-IR study: part II: skin dose. *J Vasc Interv Radiol.*
2690 2003;14:977-90.
- 2691 123. Komemushi A, Suzuki S, Sano A, Kanno S, Kariya S, Nakatani M, et al. Radiation dose of nurses
2692 during IR procedures: a controlled trial evaluating operator alerts before nursing tasks. *J Vasc Interv*
2693 *Radiol.* 2014;25:1195-9.
- 2694 124. Cameron J. Radiation dosimetry. *Environ Health Perspect.* 1991;91:45-8.
- 2695 125. Poudel S, Weir L, Dowling D, Medich DC. Changes in Occupational Radiation Exposures after
2696 Incorporation of a Real-time Dosimetry System in the Interventional Radiology Suite. *Health Phys.*
2697 2016;111:S166-71.
- 2698 126. Miljanic S, Knezevic Z, Stuhec M, Ranogajec-Komor M, Krpan K, Vekic B. Energy dependence
2699 of new thermoluminescent detectors in terms of HP(10) values. *Radiat Prot Dosimetry.*
2700 2003;106:253-6.

- 2701 127. Ito H, Kobayashi I, Watanabe K, Ochi S, Yanagawa N. Evaluation of scattered radiation from
2702 fluoroscopy using small OSL dosimeters. *Radiol Phys Technol.* 2019;12:393-400.
- 2703 128. Chida K, Kato M, Inaba Y, Kobayashi R, Nakamura M, Abe Y, et al. Real-time patient radiation
2704 dosimeter for use in interventional radiology. *Phys Med.* 2016;32:1475-8.
- 2705 129. Inaba Y, Nakamura M, Chida K, Zuguchi M. Effectiveness of a novel real-time dosimeter in
2706 interventional radiology: a comparison of new and old radiation sensors. *Radiol Phys Technol.*
2707 2018;11:445-50.
- 2708 130. Baptista M, Figueira C, Teles P, Cardoso G, Zankl M, Vaz P. Assessment of the occupational
2709 exposure in real time during interventional cardiology procedures. *Radiat Prot Dosimetry.*
2710 2015;165:304-9.
- 2711 131. Baumann F, Katzen BT, Carelsen B, Diehm N, Benenati JF, Pena CS. The Effect of Realtime
2712 Monitoring on Dose Exposure to Staff Within an Interventional Radiology Setting. *Cardiovasc*
2713 *Intervent Radiol.* 2015;38:1105-11.
- 2714 132. Muller MC, Welle K, Strauss A, Naehle PC, Pennekamp PH, Weber O, et al. Real-time
2715 dosimetry reduces radiation exposure of orthopaedic surgeons. *Orthop Traumatol Surg Res.*
2716 2014;100:947-51.
- 2717 133. Bogaert E, Bacher K, Thierens H. A large-scale multicentre study in Belgium of dose area
2718 product values and effective doses in interventional cardiology using contemporary X-ray equipment.
2719 *Radiat Prot Dosimetry.* 2008;128:312-23.
- 2720 134. Sailer AM, Vergoossen L, Paulis L, van Zwam WH, Das M, Wildberger JE, et al. Personalized
2721 Feedback on Staff Dose in Fluoroscopy-Guided Interventions: A New Era in Radiation Dose
2722 Monitoring. *Cardiovasc Intervent Radiol.* 2017;40:1756-62.

- 2723 135. Borrego D, Kitahara CM, Balter S, Yoder C. Occupational Doses to Medical Staff Performing or
2724 Assisting with Fluoroscopically Guided Interventional Procedures. *Radiology*. 2020;294:353-9.
- 2725 136. National Council on Radiation Protection and Measurements. Uncertainties in the
2726 Measurement and Dosimetry of External Radiation: Recommendations of the National Council on
2727 Radiation Protection and Measurements. NCRP Report No. 158. 2007.
- 2728 137. ICRP. Radiological Protection in Medicine. ICRP Publication 105. *Ann ICRP* 2007; 37.
- 2729 138. Hertault A, Maurel B, Midulla M, Bordier C, Desponds L, Saeed Kilani M, et al. Editor's Choice
2730 - Minimizing Radiation Exposure During Endovascular Procedures: Basic Knowledge, Literature
2731 Review, and Reporting Standards. *Eur J Vasc Endovasc Surg*. 2015;50:21-36.
- 2732 139. Resch TA, Törnqvist P, Sonesson B, Dias NV. Techniques to reduce radiation for patients and
2733 operators during aortic endografting. *J Cardiovasc Surg (Torino)*. 2016;57:178-84.
- 2734 140. Maurel B, Hertault A, Mont LSd, Cazaban S, Rinckenbach S. A Multicenter Survey of
2735 Endovascular Theatre Equipment and Radiation Exposure in France during Iliac Procedures. *Ann Vasc*
2736 *Surg*. 2017;40:50-6.
- 2737 141. Stangenberg L, Shuja F, Bom IMJvd, Alfen MHGv, Hamdan AD, Wyers MC, et al. Modern Fixed
2738 Imaging Systems Reduce Radiation Exposure to Patients and Providers. *Vasc Endovascular Surg*.
2739 2018;52:52-8.
- 2740 142. Doyen B, Maurel B, Hertault A, Vlerick P, Mastracci T, Herzeele IV, et al. Radiation Safety
2741 Performance is More than Simply Measuring Doses! Development of a Radiation Safety Rating Scale.
2742 *Cardiovasc Intervent Radiol*. 2020;43:1331-41.
- 2743 143. Dawson J, Haulon S. Radiation Stewardship: Radiation Exposure, Protection and Safety in
2744 Contemporary Endovascular Practice. In: *Mechanisms of Vascular Disease - A Reference Book for*
2745 *Vascular Specialists* Ed R Fitridge. 2nd ed. Springer Nature. 2020.

- 2746 144. Parisi MT, Bermo MS, Alessio AM, Sharp SE, Gelfand MJ, Shulkin BL. Optimization of Pediatric
2747 PET/CT. *Semin Nucl Med.* 2017;47:258-74.
- 2748 145. Killewich LA, Falls G, Mastracci TM, Brown KR. Factors affecting radiation injury. *J Vasc Surg.*
2749 2011;53:9S-14S.
- 2750 146. Brown KR, Rzucidlo E. Acute and chronic radiation injury. *J Vasc Surg.* 2011;53:15S-21S.
- 2751 147. Durán A, Hian SK, Miller DL, Heron JL, Padovani R, Vano E. Recommendations for
2752 occupational radiation protection in interventional cardiology. *Catheter Cardiovasc Interv.*
2753 2013;82:29-42.
- 2754 148. Lipsitz EC, Veith FJ, Ohki T, Heller S, Wain RA, Suggs WD, et al. Does the endovascular repair
2755 of aortoiliac aneurysms pose a radiation safety hazard to vascular surgeons? *J Vasc Surg.*
2756 2000;32:704-10.
- 2757 149. Killewich LA, Singleton TA. Governmental regulations and radiation exposure. *J Vasc Surg.*
2758 2011;53:44S-6S.
- 2759 150. Ketteler ER, Brown KR. Radiation exposure in endovascular procedures. *J Vasc Surg.*
2760 2011;53:35S-8S.
- 2761 151. Machan L. The Eyes Have It. *Tech Vasc Interv Radiol.* 2018;21:21-5.
- 2762 152. Pitton MB, Kloeckner R, Schneider J, Ruckes C, Bersch A, Düber C. Radiation exposure in
2763 vascular angiographic procedures. *J Vasc Interv Radiol.* 2012;23:1487-95.
- 2764 153. Kim KP, Miller DL, Balter S, Kleinerman RA, Linet MS, Kwon D, et al. Occupational Radiation
2765 Doses to Operators Performing Cardiac Catheterization Procedures. *Health Phys.* 2008;94:211-27.
- 2766 154. Bicknell CD. Occupational radiation exposure and the vascular interventionalist. *Eur J Vasc*
2767 *Endovasc Surg.* 2013;46:431.

- 2768 155. Lederman HM, Khademian ZP, Felice M, Hurh PJ. Dose reduction fluoroscopy in pediatrics.
2769 *Pediatr Radiol.* 2002;32:844-8.
- 2770 156. Sanchez RM, Vano E, Salinas P, Gonzalo N, Escaned J, Fernández JM. High filtration in
2771 interventional practices reduces patient radiation doses but not always scatter radiation doses. *Br J*
2772 *Radiol.* 2021;94:20200774.
- 2773 157. de Ruiter QM, Gijsberts CM, Hazenberg CE, Moll FL, van Herwaarden JA. Radiation Awareness
2774 for Endovascular Abdominal Aortic Aneurysm Repair in the Hybrid Operating Room. An Instant
2775 Patient Risk Chart for Daily Practice. *J Endovasc Ther.* 2017;24:425-34.
- 2776 158. Gentric JC, Jannin P, Trelhu B, Riffaud L, Raoult H, Ferré JC, et al. Effects of low-dose protocols
2777 in endovascular treatment of intracranial aneurysms: development of workflow task analysis during
2778 cerebral endovascular procedures. *AJR Am J Roentgenol.* 2013;201:W322-5.
- 2779 159. Baumann F, Peña C, Kloeckner R, Katzen BT, Gandhi R, Benenati JB. The Effect of a New
2780 Angiographic Imaging Technology on Radiation Dose in Visceral Embolization Procedures. *Vasc*
2781 *Endovascular Surg.* 2017;51:183-7.
- 2782 160. Ahmed TAN, Taha S. Radiation exposure, the forgotten enemy: Toward implementation of
2783 national safety program. *Egypt Heart J.* 2017;69:55-62.
- 2784 161. Read P, Meyer M-P. Restoration of Motion Picture Film. Chapter 2 Light, sound and
2785 audiovisual perception. 1st ed. Butterworth Heinemann. 2000.
- 2786 162. Miller DL, Balter S, Noonan PT, Georgia JD. Minimizing Radiation-induced Skin Injury in
2787 Interventional Radiology Procedures. *Radiology.* 2002;225:329-36.
- 2788 163. Rolls AE, Rosen S, Constantinou J, Davis M, Cole J, Desai M, et al. Introduction of a Team
2789 Based Approach to Radiation Dose Reduction in the Enhancement of the Overall Radiation Safety
2790 Profile of FEVAR. *Eur J Vasc Endovasc Surg.* 2016;52:451-7.

- 2791 164. Hirshfeld JW, Ferrari VA, Bengel FM, Bergersen L, Chambers CE, Einstein AJ, et al. 2018
 2792 ACC/HRS/NASCI/SCAI/SCCT Expert Consensus Document on Optimal Use of Ionizing Radiation
 2793 in Cardiovascular Imaging: Best Practices for Safety and Effectiveness: A Report of the American
 2794 College of Cardiology Task Force on Expert Consensus Decision Pathways. *J Am Coll Cardiol.*
 2795 2018;71:e283-e351.
- 2796 165. Patel AP, Gallacher D, Dourado R, Lyons O, Smith A, Zayed H, et al. Occupational radiation
 2797 exposure during endovascular aortic procedures. *Eur J Vasc Endovasc Surg.* 2013;46:424-30.
- 2798 166. Layton KF, Kallmes DF, Cloft HJ, Schueler BA, Sturchio GM. Radiation exposure to the primary
 2799 operator during endovascular surgical neuroradiology procedures. *AJNR Am J Neuroradiol.*
 2800 2006;27:742-3.
- 2801 167. Usai MV, Schafers J, Wunderle K, F. TG, Panuccio G. Radiation Dose Distribution in
 2802 Endovascular Aneurysm Repair in the Hybrid Operating Room According to the Specific Phases of the
 2803 Procedure. *Eur J Vasc Endovasc Surg.* 2018;56:p e17-8.
- 2804 168. Zhou W. Radiation exposure of vascular surgery patients beyond endovascular procedures. *J*
 2805 *Vasc Surg.* 2011;53:39S-43S.
- 2806 169. Sharafuddin MJ, Marjan AE. Current status of carbon dioxide angiography. *J Vasc Surg.*
 2807 2017;66:618-37.
- 2808 170. Young M, Mohan J. Carbon Dioxide Angiography. [Updated 2021 Jul 9]. In: StatPearls
 2809 [Internet]. Treasure Island (FL): StatPearls Publishing; 2021 Jan-.
 2810 <https://www.ncbi.nlm.nih.gov/books/NBK534244/>.
- 2811 171. Haqqani OP, Agarwal PK, Halin NM, lafrati MD. Defining the radiation scatter cloud in the
 2812 interventional suite. *J Vasc Surg.* 2013;58:1339-45.
- 2813 172. Miller DL. Make Radiation Protection a Habit. *Tech Vasc Interv Radiol.* 2018;21:37-42.

- 2814 173. Tonnessen BH, Pounds L. Radiation physics. *J Vasc Surg.* 2011;53:6S-8S.
- 2815 174. Lindsay BD, Eichung JO, Ambos HD, Cain ME. Radiation exposure to patients and medical
2816 personnel during radiofrequency catheter ablation for supraventricular tachycardia. *Am J Cardiol.*
2817 1992;70:218-23.
- 2818 175. Balter S. Always on My Mind. *Tech Vasc Interv Radiol.* 2018;21:26-31.
- 2819 176. Haqqani OP, Agarwal PK, Halin NM, lafrati MD. Minimizing radiation exposure to the vascular
2820 surgeon. *J Vasc Surg.* 2012;55:799-805.
- 2821 177. Gould R, McFadden SL, Sands AJ, McCrossan BA, Horn S, Prise KM, et al. Removal of scatter
2822 radiation in paediatric cardiac catheterisation: a randomised controlled clinical trial. *J Radiol Prot.*
2823 2017;37:742-60.
- 2824 178. Bang VV, Levy MS. Radiation safety with dose reduction technology: The buck stops at zero
2825 dose. *Catheter Cardiovasc Interv.* 2018;91:1200-1.
- 2826 179. Kirkwood ML, Guild JB, Arbique GM, Tsai S, Modrall JG, Anderson JA, et al. New image-
2827 processing and noise-reduction software reduces radiation dose during complex endovascular
2828 procedures. *J Vasc Surg.* 2016;64:1357-65.
- 2829 180. Strijen MJv, Grünhagen T, Mauti M, Zähringer M, Gaines PA, Robinson GJ, et al. Evaluation of
2830 a Noise Reduction Imaging Technology in Iliac Digital Subtraction Angiography: Noninferior Clinical
2831 Image Quality with Lower Patient and Scatter Dose. *J Vasc Interv Radiol.* 2015;26:642-50.e1.
- 2832 181. Miller C, Kendrick D, Shevitz A, Kim A, Baele H, Jordan D, et al. Evaluating strategies for
2833 reducing scattered radiation in fixed-imaging hybrid operating suites. *J Vasc Surg.* 2018;67:1227-33.
- 2834 182. Stansfield T, Parker R, Masson N, Lewis D. The Endovascular Preprocedural Run Through and
2835 Brief: A Simple Intervention to Reduce Radiation Dose and Contrast Load in Endovascular Aneurysm
2836 Repair. *Vasc Endovascular Surg.* 2016;50:241-6.

- 2837 183. Kakkos SK, Tsolakis IA. Commentary on “Pre-operative Simulation of the Appropriate C-Arm
2838 Position Using Computed Tomography Post-Processing Software Reduces Radiation and Contrast
2839 Medium Exposure During EVAR Procedures”. *Eur J Vasc Endovasc Surg.* 2017;53:275.
- 2840 184. Stahlberg E, Planert M, Panagiotopoulos N, Horn M, Wiedner M, Kleemann M, et al. Pre-
2841 operative Simulation of the Appropriate C-arm Position Using Computed Tomography Post-
2842 processing Software Reduces Radiation and Contrast Medium Exposure During EVAR Procedures. *Eur*
2843 *J Vasc Endovasc Surg.* 2017;53:269-74.
- 2844 185. Molinari GJ, Guillaumon AT, Dalbem AM. Efficacy Analysis of a Script-based Guide for EVAR
2845 Execution: is it Possible to Reduce Patient Exposure to Contrast, Operative Time and Blood Loss even
2846 when Advanced Technologies are not Available? *Braz J Cardiovasc Surg.* 2015;30:650-6.
- 2847 186. Molinari GP. About Image Manipulation of the CTA on Software to Simulate the Appropriate
2848 Intra-operative C-arm Position. *Eur J Vasc Endovasc Surg.* 2018;55:902-3.
- 2849 187. Hua L, Doan K, Bajic N, Fitridge R, Dawson J. Procedural Benefits of Three-Dimensional Image
2850 Fusion Angiography During EVAR Are Associated With Improved Postoperative Outcomes. *J Vasc*
2851 *Surg.* 2015;62:536-7.
- 2852 188. Sailer AM, Haan MWd, Peppelenbosch AG, Jacobs MJ, Wildberger JE, Schurink GWH. CTA
2853 with fluoroscopy image fusion guidance in endovascular complex aortic aneurysm repair. *Eur J Vasc*
2854 *Endovasc Surg.* 2014;47:349-56.
- 2855 189. Gonçalves FB. Alas, ALARA! Why the (con)fusion? *Eur J Vasc Endovasc Surg.* 2018;56:434.
- 2856 190. Maurel B, Martin-Gonzalez T, Chong D, Irwin A, Guimbreti re G, Davis M, et al. A prospective
2857 observational trial of fusion imaging in infrarenal aneurysms. *J Vasc Surg.* 2018;68:1706-13.e1.

- 2858 191. Dias NV, Billberg H, Sonesson B, Törnqvist P, Resch T, Kristmundsson T. The effects of
2859 combining fusion imaging, low-frequency pulsed fluoroscopy, and low-concentration contrast agent
2860 during endovascular aneurysm repair. *J Vasc Surg.* 2016;63:1147-55.
- 2861 192. McNally MM, Scali ST, Feezor RJ, Neal D, Huber TS, Beck AW. Three-dimensional fusion
2862 computed tomography decreases radiation exposure, procedure time, and contrast use during
2863 fenestrated endovascular aortic repair. *J Vasc Surg.* 2015;61:309-16.
- 2864 193. Ahmad W, Obeidi Y, Majd P, Brunkwall JS. The 2D-3D Registration Method in Image Fusion Is
2865 Accurate and Helps to Reduce the Used Contrast Medium, Radiation, and Procedural Time in
2866 Standard EVAR Procedures. *Ann Vasc Surg.* 2018;51:177-86.
- 2867 194. Goudekting SR, Heinen SGH, Ünlü Ç, Heuvel DAFvd, Vries J-PPMd, Strijen MJv, et al. Pros
2868 and Cons of 3D Image Fusion in Endovascular Aortic Repair: A Systematic Review and Meta-analysis. *J*
2869 *Endovasc Ther.* 2017;24:595-603.
- 2870 195. Edsfeldt A, Sonesson B, Rosén H, Petri MH, Hongku K, Resch T, et al. Validation of a New
2871 Method for 2D Fusion Imaging Registration in a System Prepared Only for 3D. *J Endovasc Ther.*
2872 2020;27:468-72.
- 2873 196. Carrell TWG, Modarai B, Brown JRI, Penney GP. Feasibility and Limitations of an Automated
2874 2D-3D Rigid Image Registration System for Complex Endovascular Aortic Procedures. *J Endovasc*
2875 *Ther.* 2010;17:527-33.
- 2876 197. Southerland KW, Nag U, Turner M, Gilmore B, McCann R, Long C, et al. IF09. Image-Based
2877 Three-Dimensional Fusion Computed Tomography Decreases Radiation Exposure, Fluoroscopy Time,
2878 and Procedure Time During Endovascular Aortic Aneurysm Repair. *J Vasc Surg.* 2018;67:e61.
- 2879 198. de Ruiter QM, Reitsma JB, Moll FL, van Herwaarden JA. Meta-analysis of Cumulative
2880 Radiation Duration and Dose During EVAR Using Mobile, Fixed, or Fixed/3D Fusion C-Arms. *J*
2881 *Endovasc Ther.* 2016;23:944-56.

- 2882 199. Mougin J, Louis N, Maupas E, Goueffic Y, Fabre D, Haulon S. Fusion imaging guidance for
2883 endovascular recanalization of peripheral occlusive disease. *J Vasc Surg.* 2022;75:610-7.
- 2884 200. Livingstone RS, Chase D, Varghese A, George PV, George OK. Transition from image
2885 intensifier to flat panel detector in interventional cardiology: Impact of radiation dose. *J Med Phys.*
2886 2015;40:24-8.
- 2887 201. Bokou C, Schreiner-Karoussou A, Breisch R, Beissel J. Changing from image intensifier to flat
2888 detector technology for interventional cardiology procedures: a practical point of view. *Radiat Prot*
2889 *Dosimetry.* 2008;129:83-6.
- 2890 202. Prieto C, Vano E, Fernandez JM, Martinez D, Sanchez R. Increases in patient doses need to be
2891 avoided when upgrading interventional cardiology systems to flat detectors. *Radiat Prot Dosimetry.*
2892 2011;147:83-5.
- 2893 203. Tsapaki V, Kottou S, Kollaros N, Dafnomili P, Koutelou M, Vano E, et al. Comparison of a
2894 conventional and a flat-panel digital system in interventional cardiology procedures. *Br J Radiol.*
2895 2004;77:562-7.
- 2896 204. Wiesinger B, Kirchner S, Blumenstock G, Herz K, Schmehl J, Claussen CD, et al. Difference in
2897 dose area product between analog image intensifier and digital flat panel detector in peripheral
2898 angiography and the effect of BMI. *Rofo.* 2013;185:153-9.
- 2899 205. Axelsson B. Optimisation in fluoroscopy. *Biomed Imaging Interv J.* 2007;3:e47.
- 2900 206. Wiesinger B, Stütz A, Schmehl J, Claussen CD, Wiskirchen J. Comparison of Digital Flat-Panel
2901 Detector and Conventional Angiography Machines: Evaluation of Stent Detection Rates, Visibility
2902 Scores, and Dose-Area Products. *AJR Am J Roentgenol.* 2012;198:946-54.

- 2903 207. Spira D, Kirchner S, Blumenstock G, Herz K, Ketelsen D, Wiskirchen J, et al. Therapeutic
 2904 angiographic procedures: differences in dose area product between analog image intensifier and
 2905 digital flat panel detector. *Acta Radiol.* 2015;57:587-94.
- 2906 208. Kuon E, Weitmann K, Hoffmann W, Dorr M, Reffellmann T, Hummel A, et al. Efficacy of a
 2907 minicourse in radiation-reducing techniques in invasive cardiology: a multicenter field study. *JACC*
 2908 *Cardiovasc Interv.* 2014;7:382-90.
- 2909 209. Suzuki S, Furui S, Kobayashi I, Yamauchi T, Kohtake H, Takeshita K, et al. Radiation Dose to
 2910 Patients and Radiologists During Transcatheter Arterial Embolization: Comparison of a Digital Flat-
 2911 Panel System and Conventional Unit. *AJR Am J Roentgenol.* 2005;185:855-9.
- 2912 210. Chida K, Inaba Y, Saito H, Ishibashi T, Takahashi S, Kohzuki M, et al. Radiation Dose of
 2913 Interventional Radiology System Using a Flat-Panel Detector. *AJR Am J Roentgenol.* 2009;193:1680-5.
- 2914 211. Dragusin O, Breisch R, Bokou C, Beissel J. Does a flat panel detector reduce the patient
 2915 radiation dose in interventional cardiology? *Radiat Prot Dosimetry.* 2010;139:266-70.
- 2916 212. Wang J, Blackburn TJ. The AAPM/RSNA Physics Tutorial for Residents: X-ray Image
 2917 Intensifiers for Fluoroscopy. *Radiographics.* 2000;20:1471-7.
- 2918 213. SUNY Upstate Medical University, Syracuse, NY. Radiology. The Image Intensifier (II).
 2919 <http://www.upstate.edu/radiology/education/rsna/fluoro/iisize.php> (Accessed 13 Dec 2020).
- 2920 214. Hasegawa K, Umemoto N, Inoue S, Iio Y, Shibata N, Mizutani T, et al. Digital zoom is a useful,
 2921 simple, and cost-effective method of reducing radiation exposure in percutaneous coronary
 2922 intervention. *Cardiovasc Interv Ther.* 2020;35:353-60.
- 2923 215. Kato M, Chida K, Yoshida K, Sasaki F, Sasaki M, Oosaka H, et al. Reduction Method of
 2924 Patients' Radiation Dose Considering the Size of Field of View with a Digital Cine X-ray System
 2925 Loading a Flat-panel Detector. *Japanese Journal of Radiological Technology.* 2011;67:1443-7.

- 2926 216. Chapple C-L, Bradley A, Murray M, Orr P, Reay J, Riley P, et al. Radiation Safety Culture in the
2927 UK Medical Sector: A Top to Bottom Strategy. *Radiat Prot Dosimetry*. 2016;173:80-6.
- 2928 217. Beathard GA, Urbanes A, Litchfield T. Radiation Dose Associated with Dialysis Vascular Access
2929 Interventional Procedures in the Interventional Nephrology Facility. *Semin Dial*. 2013;26:503-10.
- 2930 218. Hertault A, Rhee R, Antoniou GA, Adam D, Tonda H, Rousseau H, et al. Radiation Dose
2931 Reduction During EVAR: Results from a Prospective Multicentre Study (The REVAR Study). *Eur J Vasc*
2932 *Endovasc Surg*. 2018;56:426-33.
- 2933 219. Domingos LF, García EMSN, Castillo DG, Ruiz CF, Fernández IE, Puerta CV. Radioprotection
2934 Measures during the Learning Curve with Hybrid Operating Rooms. *Ann Vasc Surg*. 2018;50:253-8.
- 2935 220. Maurel B, Sobocinski J, Perini P, Guillou M, Midulla M, Azzaoui R, et al. Evaluation of
2936 Radiation during EVAR Performed on a Mobile C-arm. *Eur J Vasc Endovasc Surg*. 2012;43:16-21.
- 2937 221. Bruschi A, Michelagnoli S, Chisci E, Mazzocchi S, Panci S, Didona A, et al. A comparison study
2938 of radiation exposure to patients during EVAR and Dyna CT in an angiosuite vs. an operating theatre.
2939 *Radiat Prot Dosimetry*. 2015;163:491-8.
- 2940 222. Varu VN, Greenberg JI, Lee JT. Improved Efficiency and Safety for EVAR with Utilization of a
2941 Hybrid Room. *Eur J Vasc Endovasc Surg*. 2013;46:675-9.
- 2942 223. Fossaceca R, Brambilla M, Guzzardi G, Cerini P, Renghi A, Valzano S, et al. The impact of
2943 radiological equipment on patient radiation exposure during endovascular aortic aneurysm repair.
2944 *Eur Radiol*. 2012;22:2424-31.
- 2945 224. Kendrick DE, Miller CP, Moorehead PA, Kim AH, Baele HR, Wong VL, et al. Comparative
2946 occupational radiation exposure between fixed and mobile imaging systems. *J Vasc Surg*.
2947 2016;63:190-7.

- 2948 225. Rehman ZU, Choksy S, Howard A, Carter J, Kyriakidis K, Elizabeth D, et al. Comparison of
 2949 Patient Radiation Dose and Contrast Use during EVAR in a Dedicated Hybrid Vascular OR and Mobile
 2950 Imaging. *Ann Vasc Surg.* 2019;61:278-83.
- 2951 226. Hertault A, Bianchini A, Amiot S, Chenorhokian H, Laurent-Daniel F, Chakfé N, et al.
 2952 Comprehensive Literature Review of Radiation Levels During Endovascular Aortic Repair in Cathlabs
 2953 and Operating Theatres. *Eur J Vasc Endovasc Surg.* 2020;60:374-85.
- 2954 227. Guillou M, Maurel B, Necib H, Vent P-A, Costargent A, Chaillou P, et al. Comparison of
 2955 Radiation Exposure during Endovascular Treatment of Peripheral Arterial Disease with Flat-Panel
 2956 Detectors on Mobile C-arm versus Fixed Systems. *Ann Vasc Surg.* 2018;47:104-13.
- 2957 228. McAnelly S-L, Kelleher D, Ibrahim R, Antoniou GA. Does the use of a hybrid theatre in
 2958 vascular surgery result in improved clinical outcomes and radiation protection? *Int Angiol.*
 2959 2017;36:289-92.
- 2960 229. Kaplan DJ, Patel JN, Liporace FA, Yoon RS. Intraoperative radiation safety in orthopaedics: a
 2961 review of the ALARA (As low as reasonably achievable) principle. *Patient Saf Surg.* 2016;10:27.
- 2962 230. Peach G, Sinha S, Black SA, Morgan RA, Loftus IM, Thompson MM, et al. Operator-controlled
 2963 imaging significantly reduces radiation exposure during EVAR. *Eur J Vasc Endovasc Surg.*
 2964 2012;44:395-8.
- 2965 231. Yeo CH, Gordon R, Nusem I. Improving operating theatre communication between the
 2966 orthopaedics surgeon and radiographer. *ANZ J Surg.* 2014;84:316-9.
- 2967 232. Agarwal S, Parashar A, Bajaj NS, Khan I, Ahmad I, Heupler FA, et al. Relationship of Beam
 2968 Angulation and Radiation Exposure in the Cardiac Catheterization Laboratory. *JACC Cardiovasc Interv.*
 2969 2014;7:558-66.

- 2970 233. Kirkwood ML, Arbique GM, Guild JB, Timaran C, Chung J, Anderson JA, et al. Surgeon
2971 education decreases radiation dose in complex endovascular procedures and improves patient
2972 safety. *J Vasc Surg.* 2013;58:715-21.
- 2973 234. Oi I. Remote Contrast Injector in ERCP for Protection from X-Ray Exposure. *Endoscopy.*
2974 1982;14:180-1.
- 2975 235. Goss JE, Ramo BW, Raff GL, Maddoux GL, Heuser RR, Shadoff N, et al. Power injection of
2976 contrast media during percutaneous transluminal coronary artery angioplasty. *Cathet Cardiovasc*
2977 *Diagn.* 1989;16:195-8.
- 2978 236. Santen BC, Kan K, Velthuyse HJM, Julius HW, Kan C. Exposure of the Radiologist to Scattered
2979 Radiation during Angiography. *Radiology.* 1975;115:447-50.
- 2980 237. Marque N, Jégou A, Varenne O, Salengro E, Allouch P, Margot O, et al. Impact of an extension
2981 tube on operator radiation exposure during coronary procedures performed through the radial
2982 approach. *Arch Cardiovasc Dis.* 2009;102:749-54.
- 2983 238. Larsen AS, Osteras BH. Step back from the patient: reduction of radiation dose to the
2984 operator by the systematic use of an automatic power injector for contrast media in an
2985 interventional angiography suite. *Acta Radiol.* 2012;53:330-4.
- 2986 239. Meghazifene A, Vano E, Le Heron J, Cheung KY. Roles and responsibilities of medical physicists
2987 in radiation protection. *Eur J Radiol.* 2010;76:24-7.
- 2988 240. Badawy MK, Deb P, Chan R, Farouque O. A Review of Radiation Protection Solutions for the
2989 Staff in the Cardiac Catheterisation Laboratory. *Heart Lung Circ.* 2016;25:961-7.
- 2990 241. <https://www.iaea.org> IAEA.
- 2991 242. Mori H, Koshida K, Ishigamori O, Matsubara K. Evaluation of the effectiveness of X-ray
2992 protective aprons in experimental and practical fields. *Radiol Phys Technol.* 2014;7:158-66.

- 2993 243. Chou LB, Chandran S, Harris AH, Tung J, Butler LM. Increased breast cancer prevalence
2994 among female orthopedic surgeons. *J Womens Health (Larchmt)*. 2012;21:683-9.
- 2995 244. Valone LC, Chambers M, Lattanza L, James MA. Breast Radiation Exposure in Female
2996 Orthopaedic Surgeons. *J Bone Joint Surg Am*. 2016;98:1808-13.
- 2997 245. Van Nortwick SS, Leonard DA, Finlay AK, Chou L, Valone LC. Methods for Reducing
2998 Intraoperative Breast Radiation Exposure of Orthopaedic Surgeons. *J Bone Joint Surg Am*.
2999 2021;103:1646-51.
- 3000 246. Livingstone RS, Varghese A, Keshava SN. A Study on the Use of Radiation-Protective Apron
3001 among Interventionists in Radiology. *J Clin Imaging Sci*. 2018;8:34.
- 3002 247. Klein LW, Miller DL, Balter S, Laskey W, Haines D, Norbash A, et al. Occupational health
3003 hazards in the interventional laboratory: time for a safer environment. *J Vasc Interv Radiol*.
3004 2009;20:147-52.
- 3005 248. Livingstone RS, Varghese A. A simple quality control tool for assessing integrity of lead
3006 equivalent aprons. *Indian J Radiol Imaging*. 2018;28:258-62.
- 3007 249. Tayebi M, Shooli FS, Saeedi-Moghadam M. Evaluation of the scattered radiations of lead and
3008 lead-free aprons in diagnostic radiology by MCNPX. *Technol Health Care*. 2017;25:513-20.
- 3009 250. Johansen S, Hauge IHR, Hogg P, England A, Lanca L, Gunn C, et al. Are Antimony-Bismuth
3010 Aprons as Efficient as Lead Rubber Aprons in Providing Shielding against Scattered Radiation? *J Med*
3011 *Imaging Radiat Sci*. 2018;49:201-6.
- 3012 251. Kazempour M, Saeedimoghadam M, Shekoohi Shooli F, Shokrpour N. Assessment of the
3013 Radiation Attenuation Properties of Several Lead Free Composites by Monte Carlo Simulation. *J*
3014 *Biomed Phys Eng*. 2015;5:67-76.

- 3015 252. Finnerty M, Brennan PC. Protective aprons in imaging departments: manufacturer stated
3016 lead equivalence values require validation. *Eur Radiol.* 2005;15:1477-84.
- 3017 253. Fakhoury E, Provencher JA, Subramaniam R, Finlay DJ. Not all lightweight lead aprons and
3018 thyroid shields are alike. *J Vasc Surg.* 2019;70:246-50.
- 3019 254. Lu H, Boyd C, Dawson J. Lightweight Lead Aprons: The Emperor's New Clothes in the
3020 Angiography Suite? *Eur J Vasc Endovasc Surg.* 2019;57:730-9.
- 3021 255. Pichler T, Schopf T, Ennemoser O. [Radiation protection clothing in X-ray diagnostics -
3022 comparison of attenuation equivalents in narrow beam and inverse broad-beam geometry]. *Rofo.*
3023 2011;183:470-6.
- 3024 256. Eder H, Panzer W, Schofer H. [Is the lead-equivalent suited for rating protection properties of
3025 lead-free radiation protective clothing?]. *Rofo.* 2005;177:399-404.
- 3026 257. Matsuda M, Suzuki T. Evaluation of lead aprons and their maintenance and management at
3027 our hospital. *J Anesth.* 2016;30:518-21.
- 3028 258. Stam W, Pillay M. Inspection of lead aprons: a practical rejection model. *Health Phys.*
3029 2008;95 Suppl 2:S133-6.
- 3030 259. Oyar O, Kislalioglu A. How protective are the lead aprons we use against ionizing radiation?
3031 *Diagn Interv Radiol.* 2012;18:147-52.
- 3032 260. Lambert K, McKeon T. Inspection of lead aprons: criteria for rejection. *Health Phys.*
3033 2001;80:S67-9.
- 3034 261. Burns KM, Shoag JM, Kahlon SS, Parsons PJ, Bijur PE, Taragin BH, et al. Lead Aprons Are a
3035 Lead Exposure Hazard. *J Am Coll Radiol.* 2017;14:641-7.
- 3036 262. Ron E, Lubin JH, Shore RE, Mabuchi K, Modan B, Pottern LM, et al. Thyroid cancer after
3037 exposure to external radiation: a pooled analysis of seven studies. *Radiat Res.* 1995;141:259-77.

- 3038 263. Whitby M, Martin CJ. Radiation doses to the legs of radiologists performing interventional
3039 procedures: are they a cause for concern? *Br J Radiol.* 2003;76:321-7.
- 3040 264. Hammer GP, Scheidemann-Wesp U, Samkange-Zeeb F, Wicke H, Neriishi K, Blettner M.
3041 Occupational exposure to low doses of ionizing radiation and cataract development: a systematic
3042 literature review and perspectives on future studies. *Radiat Environ Biophys.* 2013;52:303-19.
- 3043 265. Coppeta L, Pietroiusti A, Neri A, Spataro A, De Angelis E, Perrone S, et al. Risk of radiation-
3044 induced lens opacities among surgeons and interventional medical staff. *Radiol Phys Technol.*
3045 2019;12:26-9.
- 3046 266. Thome C, Chambers DB, Hooker AM, Thompson JW, Boreham DR. Deterministic Effects to
3047 the Lens of the Eye Following Ionizing Radiation Exposure: is There Evidence to Support a Reduction
3048 in Threshold Dose? *Health Phys.* 2018;114:328-43.
- 3049 267. Seals KF, Lee EW, Cagnon CH, Al-Hakim RA, Kee ST. Radiation-Induced Cataractogenesis: A
3050 Critical Literature Review for the Interventional Radiologist. *Cardiovasc Intervent Radiol.*
3051 2016;39:151-60.
- 3052 268. Hamada N, Fujimichi Y. Role of carcinogenesis related mechanisms in cataractogenesis and
3053 its implications for ionizing radiation cataractogenesis. *Cancer Lett.* 2015;368:262-74.
- 3054 269. Matsubara K, Takei Y, Mori H, Kobayashi I, Noto K, Igarashi T, et al. A multicenter study of
3055 radiation doses to the eye lenses of medical staff performing non-vascular imaging and
3056 interventional radiology procedures in Japan. *Phys Med.* 2020;74:83-91.
- 3057 270. Bitarafan Rajabi A, Noohi F, Hashemi H, Haghjoo M, Miraftab M, Yaghoobi N, et al. Ionizing
3058 radiation-induced cataract in interventional cardiology staff. *Res Cardiovasc Med.* 2015;4:e25148.

- 3059 271. Maeder M, Brunner-La Rocca HP, Wolber T, Ammann P, Roelli H, Rohner F, et al. Impact of a
3060 lead glass screen on scatter radiation to eyes and hands in interventional cardiologists. *Catheter*
3061 *Cardiovasc Interv.* 2006;67:18-23.
- 3062 272. Kirkwood ML, Klein A, Guild J, Arbique G, Xi Y, Tsai S, et al. Novel modification to leaded
3063 eyewear results in significant operator eye radiation dose reduction. *J Vasc Surg.* 2020;72:2139-44.
- 3064 273. Cousin AJ, Lawdahl RB, Chakraborty DP, Koehler RE. The case for radioprotective
3065 eyewear/facewear. Practical implications and suggestions. *Invest Radiol.* 1987;22:688-92.
- 3066 274. Vano E, Gonzalez L, Guibelalde E, Fernandez JM, Ten JJ. Radiation exposure to medical staff in
3067 interventional and cardiac radiology. *Br J Radiol.* 1998;71:954-60.
- 3068 275. Wagner LK, Mulhern OR. Radiation-attenuating surgical gloves: effects of scatter and
3069 secondary electron production. *Radiology.* 1996;200:45-8.
- 3070 276. Kamusella P, Scheer F, Ludtke CW, Wiggermann P, Wissgott C, Andresen R. Interventional
3071 Angiography: Radiation Protection for the Examiner by using Lead-free Gloves. *J Clin Diagn Res.*
3072 2017;11:TC26-TC9.
- 3073 277. Seto AH, Abu-Fadel MS, Sparling JM, Zacharias SJ, Daly TS, Harrison AT, et al. Real-time
3074 ultrasound guidance facilitates femoral arterial access and reduces vascular complications: FAUST
3075 (Femoral Arterial Access With Ultrasound Trial). *JACC Cardiovasc Interv.* 2010;3:751-8.
- 3076 278. Slattery MM, Goh GS, Power S, Given MF, McGrath FP, Lee MJ. Comparison of ultrasound-
3077 guided and fluoroscopy-assisted antegrade common femoral artery puncture techniques. *Cardiovasc*
3078 *Intervent Radiol.* 2015;38:579-82.
- 3079 279. Sobolev M, Slovut DP, Lee Chang A, Shiloh AL, Eisen LA. Ultrasound-Guided Catheterization of
3080 the Femoral Artery: A Systematic Review and Meta-Analysis of Randomized Controlled Trials. *J*
3081 *Invasive Cardiol.* 2015;27:318-23.

- 3082 280. Stone P, Campbell J, Thompson S, Walker J. A prospective, randomized study comparing
3083 ultrasound versus fluoroscopic guided femoral arterial access in noncardiac vascular patients. *J Vasc*
3084 *Surg.* 2020;72:259-67.
- 3085 281. Finkelstein MM. Is brain cancer an occupational disease of cardiologists? *Can J Cardiol.*
3086 1998;14:1385-8.
- 3087 282. Hardell L, Mild KH, Pålsson A, Hallquist A. Ionizing radiation, cellular telephones and the risk
3088 for brain tumours. *Eur J Cancer Prev.* 2001;10:523-375.
- 3089 283. Kuon E, Birkel J, Schmitt M, Dahm JB. Radiation exposure benefit of a lead cap in invasive
3090 cardiology. *Heart.* 2003;89:1205-10.
- 3091 284. Karadag B, Ikitimur B, Durmaz E, Avci BK, Cakmak HA, Cosansu K, et al. Effectiveness of a lead
3092 cap in radiation protection of the head in the cardiac catheterisation laboratory. *EuroIntervention.*
3093 2013;9:754-6.
- 3094 285. Uthoff H, Pena C, West J, Contreras F, Benenati JF, Katzen BT. Evaluation of novel disposable,
3095 light-weight radiation protection devices in an interventional radiology setting: a randomized
3096 controlled trial. *AJR Am J Roentgenol.* 2013;200:915-20.
- 3097 286. Uthoff H, Quesada R, Roberts JS, Baumann F, Scherthaner M, Zaremski L, et al.
3098 Radioprotective lightweight caps in the interventional cardiology setting: a randomised controlled
3099 trial (PROTECT). *EuroIntervention.* 2015;11:53-9.
- 3100 287. Chohan MO, Sandoval D, Buchan A, Murray-Krezan C, Taylor CL. Cranial radiation exposure
3101 during cerebral catheter angiography. *J Neurointerv Surg.* 2014;6:633-6.
- 3102 288. Alazzoni A, Gordon CL, Syed J, Natarajan MK, Rokoss M, Schwalm JD, et al. Randomized
3103 Controlled Trial of Radiation Protection With a Patient Lead Shield and a Novel, Nonlead Surgical Cap

- 3104 for Operators Performing Coronary Angiography or Intervention. *Circ Cardiovasc Interv.*
 3105 2015;8:e002384.
- 3106 289. Mayr NP, Wiesner G, Kretschmer A, Bronner J, Hoedlmoser H, Husser O, et al. Assessing the
 3107 level of radiation experienced by anesthesiologists during transfemoral Transcatheter Aortic Valve
 3108 Implantation and protection by a lead cap. *PLoS One.* 2019;14:e0210872.
- 3109 290. Fetterly K, Schueler B, Grams M, Sturchio G, Bell M, Gulati R. Head and Neck Radiation Dose
 3110 and Radiation Safety for Interventional Physicians. *JACC Cardiovasc Interv.* 2017;10:520-8.
- 3111 291. Sans Merce M, Korchi AM, Kobzeva L, Damet J, Erceg G, Marcos Gonzalez A, et al. The value
 3112 of protective head cap and glasses in neurointerventional radiology. *J Neurointerv Surg.* 2016;8:736-
 3113 40.
- 3114 292. Kirkwood ML, Arbique GM, Guild JB, Zeng K, Xi Y, Rectenwald J, et al. Radiation brain dose to
 3115 vascular surgeons during fluoroscopically guided interventions is not effectively reduced by wearing
 3116 lead equivalent surgical caps. *J Vasc Surg.* 2018;68:567-71.
- 3117 293. Fetterly KA, Magnuson DJ, Tannahill GM, Hindal MD, Mathew V. Effective use of radiation
 3118 shields to minimize operator dose during invasive cardiology procedures. *JACC Cardiovasc Interv.*
 3119 2011;4:1133-9.
- 3120 294. Marichal DA, Anwar T, Kirsch D, Clements J, Carlson L, Savage C, et al. Comparison of a
 3121 suspended radiation protection system versus standard lead apron for radiation exposure of a
 3122 simulated interventionalist. *J Vasc Interv Radiol.* 2011;22:437-42.
- 3123 295. Savage C, Seale IV T, Shaw C, Angela B, Marichal D, Rees C. Evaluation of a Suspended
 3124 Personal Radiation Protection System vs. Conventional Apron and Shields in Clinical Interventional
 3125 Procedures. *Open J Radiol.* 2013;3:143-51.

- 3126 296. Haussen DC, Van Der Bom IM, Nogueira RG. A prospective case control comparison of the
3127 ZeroGravity system versus a standard lead apron as radiation protection strategy in
3128 neuroendovascular procedures. *J Neurointerv Surg*. 2016;8:1052-5.
- 3129 297. Pierno J, Hamilton C. SU-E-I-35: Experience with Th Zero Gravity Suit. *Med Phys*.
3130 2012;39:3633.
- 3131 298. Madder RD, VanOosterhout S, Mulder A, Elmore M, Campbell J, Borgman A, et al. Impact of
3132 robotics and a suspended lead suit on physician radiation exposure during percutaneous coronary
3133 intervention. *Cardiovasc Revasc Med*. 2017;18:190-6.
- 3134 299. Salcido-Rios J, McNamara DA, VanOosterhout S, VanLoo L, Redmond M, Parker JL, et al.
3135 Suspended lead suit and physician radiation doses during coronary angiography. *Catheter Cardiovasc*
3136 *Interv*. 2022;99:981-8.
- 3137 300. Thornton RH, Dauer LT, Altamirano JP, Alvarado KJ, St Germain J, Solomon SB. Comparing
3138 strategies for operator eye protection in the interventional radiology suite. *J Vasc Interv Radiol*.
3139 2010;21:1703-7.
- 3140 301. Vano E, Rm SC, Jm FS. Helping to know if you are properly protected while working in
3141 interventional cardiology. *J Radiol Prot*. 2020;40.
- 3142 302. Sukupova L, Hlavacek O, Vedlich D. Impact of the Ceiling-Mounted Radiation Shielding
3143 Position on the Physician's Dose from Scatter Radiation during Interventional Procedures. *Radiol Res*
3144 *Pract*. 2018;2018:4287973.
- 3145 303. Eder H, Seidenbusch MC, Treitl M, Gilligan P. A New Design of a Lead-Acrylic Shield for Staff
3146 Dose Reduction in Radial and Femoral Access Coronary Catheterization. *Rofo*. 2015;187:915-23.

- 3147 304. Sciahbasi A, Sarandrea A, Rigattieri S, Patrizi R, Cera M, Di Russo C, et al. Extended Protective
3148 Shield Under Table to Reduce Operator Radiation Dose in Percutaneous Coronary Procedures. *Circ*
3149 *Cardiovasc Interv.* 2019;12:e007586.
- 3150 305. Jia Q, Chen Z, Jiang X, Zhao Z, Huang M, Li J, et al. Operator Radiation and the Efficacy of
3151 Ceiling-Suspended Lead Screen Shielding during Coronary Angiography: An Anthropomorphic
3152 Phantom Study Using Real-Time Dosimeters. *Sci Rep.* 2017;7:42077.
- 3153 306. Madder RD, LaCombe A, VanOosterhout S, Mulder A, Elmore M, Parker JL, et al. Radiation
3154 Exposure Among Scrub Technologists and Nurse Circulators During Cardiac Catheterization: The
3155 Impact of Accessory Lead Shields. *JACC Cardiovasc Interv.* 2018;11:206-12.
- 3156 307. Marcusohn E, Postnikov M, Musallam A, Yalonetsky S, Mishra S, Kerner A, et al. Usefulness of
3157 Pelvic Radiation Protection Shields During Transfemoral Procedures-Operator and Patient
3158 Considerations. *Am J Cardiol.* 2018;122:1098-103.
- 3159 308. King JN, Champlin AM, Kelsey CA, Tripp DA. Using a sterile disposable protective surgical
3160 drape for reduction of radiation exposure to interventionalists. *AJR Am J Roentgenol.* 2002;178:153-
3161 7.
- 3162 309. Power S, Mirza M, Thakorlal A, Ganai B, Gavagan LD, Given MF, et al. Efficacy of a radiation
3163 absorbing shield in reducing dose to the interventionalist during peripheral endovascular procedures:
3164 a single centre pilot study. *Cardiovasc Intervent Radiol.* 2015;38:573-8.
- 3165 310. Vlastra W, Delewi R, Sjaauw KD, Beijik MA, Claessen BE, Streekstra GJ, et al. Efficacy of the
3166 RADPAD Protection Drape in Reducing Operators' Radiation Exposure in the Catheterization
3167 Laboratory: A Sham-Controlled Randomized Trial. *Circ Cardiovasc Interv.* 2017;10:e006058.
- 3168 311. Ordiales JM, Nogales JM, Vano E, Lopez-Minguez JR, Alvarez FJ, Ramos J, et al. Occupational
3169 dose reduction in cardiac catheterisation laboratory: a randomised trial using a shield drape placed
3170 on the patient. *Radiat Prot Dosimetry.* 2017;174:255-61.

- 3171 312. Politi L, Biondi-Zoccai G, Nocetti L, Costi T, Monopoli D, Rossi R, et al. Reduction of scatter
 3172 radiation during transradial percutaneous coronary angiography: a randomized trial using a lead-free
 3173 radiation shield. *Catheter Cardiovasc Interv.* 2012;79:97-102.
- 3174 313. Simons GR, Orrison WW, Jr. Use of a sterile, disposable, radiation-absorbing shield reduces
 3175 occupational exposure to scatter radiation during pectoral device implantation. *Pacing Clin*
 3176 *Electrophysiol.* 2004;27:726-9.
- 3177 314. Kloeze C, Klompenhouwer EG, Brands PJ, van Sambeek MR, Cuypers PW, Teijink JA. Editor's
 3178 choice--Use of disposable radiation-absorbing surgical drapes results in significant dose reduction
 3179 during EVAR procedures. *Eur J Vasc Endovasc Surg.* 2014;47:268-72.
- 3180 315. Fattal P, Goldstein JA. A novel complete radiation protection system eliminates physician
 3181 radiation exposure and leaded aprons. *Catheter Cardiovasc Interv.* 2013;82:11-6.
- 3182 316. Iqtidar AF, Jeon C, Rothman R, Snead R, Pyne CT. Reduction in operator radiation exposure
 3183 during transradial catheterization and intervention using a simple lead drape. *Am Heart J.*
 3184 2013;165:293-8.
- 3185 317. Musallam A, Volis I, Dadaev S, Abergel E, Soni A, Yalonetsky S, et al. A randomized study
 3186 comparing the use of a pelvic lead shield during trans-radial interventions: Threefold decrease in
 3187 radiation to the operator but double exposure to the patient. *Catheter Cardiovasc Interv.*
 3188 2015;85:1164-70.
- 3189 318. Kim C, Vasaiwala S, Haque F, Pratap K, Vidovich MI. Radiation safety among cardiology
 3190 fellows. *Am J Cardiol.* 2010;106:125-8.
- 3191 319. Harris AM, Loomis J, Hopkins M, Bylund J. Assessment of Radiation Safety Knowledge Among
 3192 Urology Residents in the United States. *J Endourol.* 2019;33:492-7.

- 3193 320. Nugent M, Carmody O, Dudeney S. Radiation safety knowledge and practices among Irish
3194 orthopaedic trainees. *Ir J Med Sci.* 2015;184:369-73.
- 3195 321. Khan F, Ul-Abadin Z, Rauf S, Javed A. Awareness and attitudes amongst basic surgical trainees
3196 regarding radiation in orthopaedic trauma surgery. *Biomed Imaging Interv J.* 2010;6:e25.
- 3197 322. Bhinder J, Fakhoury E, O'Brien-Irr M, Reilly B, Dryjski M, Dosluoglu H, et al. National survey of
3198 vascular surgery residents and fellows on radiation exposure and safety practices. *J Vasc Surg.*
3199 2022;76:274-9 e1.
- 3200 323. Vlastra W, Claessen BE, Beijl MA, Sjaauw KD, Streekstra GJ, Wykrzykowska JJ, et al. Cardiology
3201 fellows-in-training are exposed to relatively high levels of radiation in the cath lab compared with
3202 staff interventional cardiologists-insights from the RECAP trial. *Neth Heart J.* 2019;27:330-3.
- 3203 324. Fetterly KA, Lennon RJ, Bell MR, Holmes DR, Jr., Rihal CS. Clinical determinants of radiation
3204 dose in percutaneous coronary interventional procedures: influence of patient size, procedure
3205 complexity, and performing physician. *JACC Cardiovasc Interv.* 2011;4:336-43.
- 3206 325. Bernardi G, Padovani R, Trianni A, Morocutti G, Spedicato L, Zanuttini D, et al. The effect of
3207 fellows' training in invasive cardiology on radiological exposure of patients. *Radiat Prot Dosimetry.*
3208 2008;128:72-6.
- 3209 326. Malik AT, Rai HH, Lakdawala RH, Noordin S. Does surgeon experience influence the amount
3210 of radiation exposure during orthopedic procedures? A systematic review. *Orthop Rev (Pavia).*
3211 2019;11:7667.
- 3212 327. Pradella M, Trumm C, Stieltjes B, Boll DT, Zech CJ, Huegli RW. Impact factors for safety,
3213 success, duration and radiation exposure in CT-guided interventions. *Br J Radiol.* 2019:20180937.

- 3214 328. Mohapatra A, Greenberg RK, Mastracci TM, Eagleton MJ, Thornsberry B. Radiation exposure
3215 to operating room personnel and patients during endovascular procedures. *Journal of vascular*
3216 *surgery*. 2013;58:702-9.
- 3217 329. Nayahangan LJ, Van Herzeele I, Konge L, Koncar I, Cieri E, Mansilha A, et al. Achieving
3218 Consensus to Define Curricular Content for Simulation Based Education in Vascular Surgery: A Europe
3219 Wide Needs Assessment Initiative. *Eur J Vasc Endovasc Surg*. 2019;58:284-91.
- 3220 330. Vassileva J, Applegate K, Paulo G, Vano E, Holmberg O. Strengthening radiation protection
3221 education and training of health professionals: conclusions from an IAEA meeting. *J Radiol Prot*.
3222 2022;42.
- 3223 331. Vano E. Mandatory radiation safety training for interventionalists: the European perspective.
3224 *Tech Vasc Interv Radiol*. 2010;13:200-3.
- 3225 332. Bartal G, Vano E, Paulo G, Miller DL. Management of patient and staff radiation dose in
3226 interventional radiology: current concepts. *Cardiovascular and interventional radiology*. 2014;37:289-
3227 98.
- 3228 333. Vano E, Rosenstein M, Liniecki J, Rehani MM, Martin CJ, Vetter RJ. ICRP Publication 113.
3229 Education and training in radiological protection for diagnostic and interventional procedures. *Ann*
3230 *ICRP*. 2009;39:7-68.
- 3231 334. ICRP. Education and Training in Radiological Protection for Diagnostic and Interventional
3232 Procedures. ICRP Publication 113. *Ann ICRP*. 2009;39.
- 3233 335. Autti T, Autti H, Vehmas T, Laitalainen V, Kivisaari L. E-learning is a well-accepted tool in
3234 supplementary training among medical doctors: an experience of obligatory radiation protection
3235 training in healthcare. *Acta Radiol*. 2007;48:508-13.

- 3236 336. Blackmon KN, Huda W, Lewis MC, Tipnis S, Mah E, Frey DG. A web based Foundations of
3237 Radiological Physics for diagnostic radiology residents. *Acad Radiol.* 2013;20:338-44.
- 3238 337. van Puyvelde L, Clarijs T, Belmans N, Coeck M. Comparing the effectiveness of learning
3239 formats in radiation protection. *J Radiol Prot.* 2021;41.
- 3240 338. Kuon E, Empen K, Robinson DM, Pfahlberg A, Gefeller O, Dahm JB. Efficiency of a minicourse
3241 in radiation reducing techniques: a pilot initiative to encourage less irradiating cardiological
3242 interventional techniques (ELICIT). *Heart.* 2005;91:1221-2.
- 3243 339. Kuon E, Weitmann K, Hoffmann W, Dorr M, Hummel A, Riad A, et al. Multicenter long-term
3244 validation of a minicourse in radiation-reducing techniques in the catheterization laboratory. *Am J*
3245 *Cardiol.* 2015;115:367-73.
- 3246 340. Azpiri-Lopez JR, Assad-Morell JL, Gonzalez-Gonzalez JG, Elizondo-Riojas G, Davila-Bortoni A,
3247 Garcia-Martinez R, et al. Effect of physician training on the X-ray dose delivered during coronary
3248 angioplasty. *J Invasive Cardiol.* 2013;25:109-13.
- 3249 341. Alahmari MAS, Sun ZH. A Systematic Review of the Efficiency of Radiation Protection Training
3250 in Raising Awareness of Medical Staff Working in Catheterisation Laboratory. *Curr Med Imaging Rev.*
3251 2015;11:200-6.
- 3252 342. Fetterly KA, Mathew V, Lennon R, Bell MR, Holmes DR, Jr., Rihal CS. Radiation dose reduction
3253 in the invasive cardiovascular laboratory: implementing a culture and philosophy of radiation safety.
3254 *JACC Cardiovasc Interv.* 2012;5:866-73.
- 3255 343. Hirshfeld JW, Jr., Ferrari VA, Bengel FM, Bergersen L, Chambers CE, Einstein AJ, et al. 2018
3256 ACC/HRS/NASCI/SCAI/SCCT Expert Consensus Document on Optimal Use of Ionizing Radiation in
3257 Cardiovascular Imaging-Best Practices for Safety and Effectiveness, Part 2: Radiological Equipment
3258 Operation, Dose-Sparing Methodologies, Patient and Medical Personnel Protection: A Report of the

- 3259 American College of Cardiology Task Force on Expert Consensus Decision Pathways. J Am Coll Cardiol.
3260 2018;71:2829-55.
- 3261 344. Giger M. Dosisintensive Röntgenuntersuchungen: Weiterbildung gemäss
3262 Strahlenschutzverordnung. Schweiz Ärztezeitung. 1998;79:413-4.
- 3263 345. Fernandez Soto JM, Vano E, Guibelalde E. Spanish experience in education and training in
3264 radiation protection in medicine. Radiat Prot Dosimetry. 2011;147:338-42.
- 3265 346. Katz A, Shtub A, Solomonica A, Poliakov A, Roguin A. Simulator training to minimize ionizing
3266 radiation exposure in the catheterization laboratory. Int J Cardiovasc Imaging. 2017;33:303-10.
- 3267 347. Patel AD, Gallagher AG, Nicholson WJ, Cates CU. Learning curves and reliability measures for
3268 virtual reality simulation in the performance assessment of carotid angiography. J Am Coll Cardiol.
3269 2006;47:1796-802.
- 3270 348. Dawson DL, Meyer J, Lee ES, Pevec WC. Training with simulation improves residents'
3271 endovascular procedure skills. J Vasc Surg. 2007;45:149-54.
- 3272 349. Kim AH, Kendrick DE, Moorehead PA, Nagavalli A, Miller CP, Liu NT, et al. Endovascular
3273 aneurysm repair simulation can lead to decreased fluoroscopy time and accurately delineate the
3274 proximal seal zone. J Vasc Surg. 2016;64:251-8.
- 3275 350. Vento V, Cencenelli L, Mascoli C, Gallitto E, Ancetti S, Faggioli G, et al. The Role of Simulation
3276 in Boosting the Learning Curve in EVAR Procedures. J Surg Educ. 2018;75:534-40.
- 3277 351. Kreiser K, Gehling KG, Ströber L, Zimmer C, Kirschke JS. Simulation Training in
3278 Neuroangiography: Transfer to Reality. Cardiovasc Intervent Radiol. 2020;43:1184-91.
- 3279 352. Rader SB, Jorgensen E, Bech B, Lonn L, Ringsted CV. Use of performance curves in estimating
3280 number of procedures required to achieve proficiency in coronary angiography. Catheter Cardiovasc
3281 Interv. 2011;78:387-93.

- 3282 353. Ramjeeawon A, Sharrock AE, Morbi A, Martin G, Riga C, Bicknell C. Using Fully-Immersive
 3283 Simulation Training with Structured Debrief to Improve Nontechnical Skills in Emergency
 3284 Endovascular Surgery. *J Surg Educ.* 2020;77:1300-11.
- 3285 354. Papatsoris AG, Shaikh T, Patel D, Bourdounis A, Bach C, Buchholz N, et al. Use of a virtual
 3286 reality simulator to improve percutaneous renal access skills: a prospective study in urology trainees.
 3287 *Urol Int.* 2012;89:185-90.
- 3288 355. Bott OJ, Dresing K, Wagner M, Raab BW, Teistler M. Informatics in radiology: use of a C-arm
 3289 fluoroscopy simulator to support training in intraoperative radiography. *Radiographics.* 2011;31:E65-
 3290 75.
- 3291 356. Faulkner AR, Bourgeois AC, Bradley YC, Hudson KB, Heidel RE, Pasciak AS. Simulation-based
 3292 educational curriculum for fluoroscopically guided lumbar puncture improves operator confidence
 3293 and reduces patient dose. *Acad Radiol.* 2015;22:668-73.
- 3294 357. Choi MH, Jung SE, Oh SN, Byun JY. Educational Effects of Radiation Reduction During
 3295 Fluoroscopic Examination of the Adult Gastrointestinal Tract. *Acad Radiol.* 2018;25:202-8.
- 3296 358. Prenner SB, Wayne DB, Sweis RN, Cohen ER, Feinglass JM, Schimmel DR. Simulation-based
 3297 education leads to decreased use of fluoroscopy in diagnostic coronary angiography. *Catheter*
 3298 *Cardiovasc Interv.* 2018;91:1054-9.
- 3299 359. De Ponti R, Marazzi R, Doni LA, Tamborini C, Ghiringhelli S, Salerno-Uriarte JA. Simulator
 3300 training reduces radiation exposure and improves trainees' performance in placing electrophysiologic
 3301 catheters during patient-based procedures. *Heart Rhythm.* 2012;9:1280-5.
- 3302 360. Popovic B, Pinelli S, Albuissou E, Metzendorf PA, Mourer B, Tran N, et al. The Simulation
 3303 Training in Coronary Angiography and Its Impact on Real Life Conduct in the Catheterization
 3304 Laboratory. *Am J Cardiol.* 2019;123:1208-13.

- 3305 361. Chaer RA, Derubertis BG, Lin SC, Bush HL, Karwowski JK, Birk D, et al. Simulation improves
 3306 resident performance in catheter-based intervention: results of a randomized, controlled study. Ann
 3307 Surg. 2006;244:343-52.
- 3308 362. Maertens H, Aggarwal R, Moreels N, Vermassen F, Van Herzeele I. A Proficiency Based
 3309 Stepwise Endovascular Curricular Training (PROSPECT) Program Enhances Operative Performance in
 3310 Real Life: A Randomised Controlled Trial. Eur J Vasc Endovasc Surg. 2017;54:387-96.
- 3311 363. Desender LM, Van Herzeele I, Lachat ML, Rancic Z, Duchateau J, Rudarakanchana N, et al.
 3312 Patient-specific Rehearsal Before EVAR: Influence on Technical and Nontechnical Operative
 3313 Performance. A Randomized Controlled Trial. Ann Surg. 2016;264:703-9.
- 3314 364. Tam MD, Latham TR, Lewis M, Khanna K, Zaman A, Parker M, et al. A Pilot Study Assessing
 3315 the Impact of 3-D Printed Models of Aortic Aneurysms on Management Decisions in EVAR Planning.
 3316 Vasc Endovascular Surg. 2016;50:4-9.
- 3317 365. Nielsen CA, Lonn L, Konge L, Taudorf M. Simulation-Based Virtual-Reality Patient-Specific
 3318 Rehearsal Prior to Endovascular Procedures: A Systematic Review. Diagnostics (Basel). 2020;10:500.
- 3319 366. Chaer RA, Derubertis BG, Lin SC, Bush HL, Karwowski JK, Birk D, et al. Simulation improves
 3320 resident performance in catheter-based intervention: results of a randomized, controlled study. Ann
 3321 Surg. 2006;244:343-52.
- 3322 367. WHO/IAEA Bonn Call for Action 2012. 10 Actions to Improve Radiation Protection in
 3323 Medicine in the Next Decade. WHO 2014. [https://www.who.int/publications/m/item/bonn-call-for-](https://www.who.int/publications/m/item/bonn-call-for-action)
 3324 action.
- 3325 368. Smith IR, Foster KA, Brighthouse RD, Cameron J, Rivers JT. The role of quantitative feedback in
 3326 coronary angiography radiation reduction. Int J Qual Health Care. 2011;23:342-8.

- 3327 369. de Ruiter QM, Moll FL, van Herwaarden JA. Current state in tracking and robotic navigation
3328 systems for application in endovascular aortic aneurysm repair. *J Vasc Surg.* 2015;61:256-64.
- 3329 370. Tystad Lund K, Tangen GA, Manstad-Hulaas F. Electromagnetic navigation versus fluoroscopy
3330 in aortic endovascular procedures: a phantom study. *Int J Comput Assist Radiol Surg.* 2017;12:51-7.
- 3331 371. Condino S, Calabro EM, Alberti A, Parrini S, Cioni R, Berchiolli RN, et al. Simultaneous tracking
3332 of catheters and guidewires: comparison to standard fluoroscopic guidance for arterial cannulation.
3333 *Eur J Vasc Endovasc Surg.* 2014;47:53-60.
- 3334 372. Jansen M, Khandige A, Kobeiter H, Vonken EJ, Hazenberg C, van Herwaarden J. Three
3335 Dimensional Visualisation of Endovascular Guidewires and Catheters Based on Laser Light instead of
3336 Fluoroscopy with Fiber Optic RealShape Technology: Preclinical Results. *Eur J Vasc Endovasc Surg.*
3337 2020;60:135-43.
- 3338 373. West K, Al-Nimer S, Goel VR, Yanof JH, Hanlon AT, Weunski CJ, et al. Three-Dimensional
3339 Holographic Guidance, Navigation, and Control (3D-GNC) for Endograft Positioning in Porcine Aorta:
3340 Feasibility Comparison With 2-Dimensional X-Ray Fluoroscopy. *J Endovasc Ther.* 2021;28:796-803.
- 3341 374. Schwein A, Kramer B, Chinnadurai P, Virmani N, Walker S, O'Malley M, et al. Electromagnetic
3342 tracking of flexible robotic catheters enables "assisted navigation" and brings automation to
3343 endovascular navigation in an in vitro study. *J Vasc Surg.* 2018;67:1274-81.
- 3344 375. van Herwaarden JA, Jansen MM, Vonken EPA, Bloemert-Tuin T, Bullens RWM, de Borst GJ, et
3345 al. First in Human Clinical Feasibility Study of Endovascular Navigation with Fiber Optic RealShape
3346 (FORS) Technology. *Eur J Vasc Endovasc Surg.* 2021;61:317-25.
- 3347 376. Panuccio G, Torrealba J, Rohlfes F, Heidemann F, Wessels B, Kolbel T. Fiber Optic RealShape
3348 (FORS) Technology for Endovascular Navigation in Severe Tortuous Vessels. *J Endovasc Ther.*
3349 2022:15266028211070969.

- 3350 377. Riga CV, Cheshire NJ, Hamady MS, Bicknell CD. The role of robotic endovascular catheters in
 3351 fenestrated stent grafting. *J Vasc Surg.* 2010;51:810-9; discussion 9-20.
- 3352 378. Cochenne F, Kobeiter H, Gohel M, Marzelle J, Desgranges P, Allaire E, et al. Feasibility and
 3353 safety of renal and visceral target vessel cannulation using robotically steerable catheters during
 3354 complex endovascular aortic procedures. *J Endovasc Ther.* 2015;22:187-93.
- 3355 379. Ambrosini P, Ruijters D, Niessen WJ, Moelker A, van Walsum T. Fully Automatic and Real-
 3356 Time Catheter Segmentation in X-Ray Fluoroscopy. *Medical Image Computing and Computer-
 3357 Assisted Intervention – MICCAI 2017. Lecture Notes in Computer Science: Springer, Cham; 2017. p.*
 3358 *577-85.*
- 3359 380. Zhou YJ, Xie XL, Zhou XH, Liu SQ, Bian GB, Hou ZG. Pyramid attention recurrent networks for
 3360 real-time guidewire segmentation and tracking in intraoperative X-ray fluoroscopy. *Comput Med*
 3361 *Imaging Graph.* 2020;83:101734.
- 3362 381. Bang JY, Hough M, Hawes RH, Varadarajulu S. Use of Artificial Intelligence to Reduce
 3363 Radiation Exposure at Fluoroscopy-Guided Endoscopic Procedures. *Am J Gastroenterol.*
 3364 *2020;115:555-61.*
- 3365 382. Abdelhalim MA, Patel A, Moquet J, Saha P, Smith A, Badie C, et al. Higher Incidence of
 3366 Chromosomal Aberrations in Operators Performing a Large Volume of Endovascular Procedures.
 3367 *Circulation.* 2022;145:1808-10.

3368

3369 APPENDICES

3370 ACKNOWLEDGEMENTS

3371

3372 On behalf of the Public and Community Oversight Group (PCOG) of the Health Protection Research

3373 Unit in Chemical and Radiation Threats and Hazards:

3374 Ian Wright

3375 John Phipps

3376 Colette Kelly

3377 Robert Goundry

3378 Eve Smyth

3379 Andrew Wood

3380 Paul Dale (also of the Scottish Environment Protection Agency)

3381

3382 On behalf of the Society and College of Radiographers Patient Advisory Group:

3383 Lynda Johnson

3384 Philip Plant

3385 Michelle Carmichael – Specialist Senior Staff Nurse Guy's and St Thomas' NHS Foundation trust

Appendices

Appendix 1: Basic knowledge related to x-rays

1.1. The physics of x-rays

X-rays are wave-like forms of electromagnetic energy that are carried by photons. They are characterized by a wavelength comprised of between 0.03 nm and 10 nm, which means they fall between gamma radiation and ultraviolet light on the electromagnetic spectrum. The energy associated with X-ray is usually measured in electro-volts (eV). The shorter the wavelength of an electromagnetic wave is, the higher the energy of the associated photons. For example, visible light photons have an energy of around 2eV, while X-ray photons have energies between 30 to 150keV.¹

X-rays are classified as ionizing radiation, meaning they have the potential to interact with biological matter when they collide with it, altering its molecular bonds and producing ionisations. The process of ionisation (in which an electron is given enough energy to break away from an atom) releases energy that can damage living tissues.

There are three possible outcomes when X-rays encounter matter (Figure A1):²

- Transmission: once the X-ray beam hits an object it passes through it without any interaction, keeping the same direction and energy.
- Diffusion/Scattering: upon hitting the object, X-rays are reflected in different directions, without energy transfer, or with partial transfer of energy and induction of ionisation – a phenomenon known as the Compton effect.
- Absorption: the energy associated with X-ray is absorbed upon passing through an object, induction atomic ionisation – this is known as the photoelectric effect.

The production of images for medical applications is dependent on the Compton and Photoelectric effect of X-rays, which relies on ionisation and, therefore, has the potential to cause biological damage.

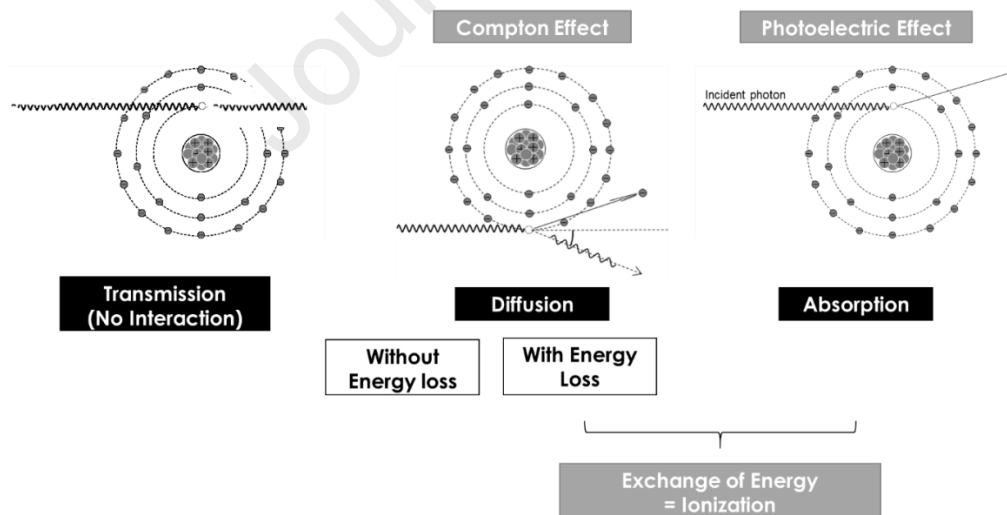


Figure A1: Main mechanisms of interaction between X-rays and matter.

1.2. X-ray production and image generation

X-ray generators (Figure A2) used in endovascular operating rooms rely on an electric current (characterized by a potential (kV)) to accelerate and induce electron collision on an anode. As much as 99% of the current's energy is transformed into heat, explaining the need for cooling systems in imaging equipment. The remaining 1% of energy is used to generate an X-ray beam that exits the X-ray tube.³

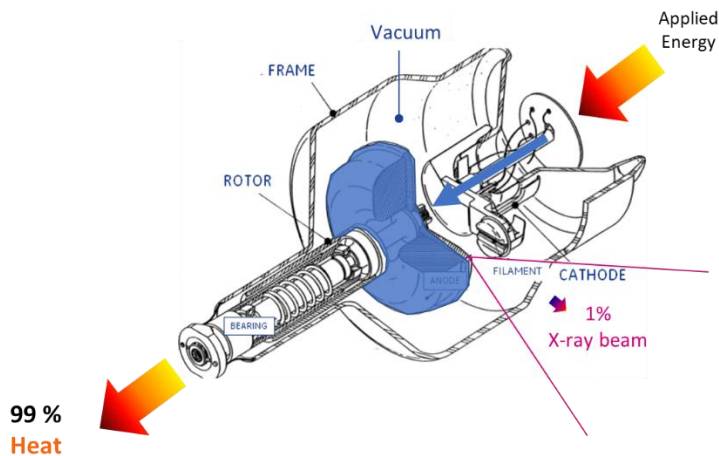


Figure A2: Example of an X-ray generator; electrons are accelerated (blue arrow) and collided on an anode (blue structure). Most of the energy is released in the form of heat, the remaining 1% forms X-rays.

The X-ray beam released travels through the operating table and the patient. Part of the beam is redirected in random directions due to the Compton effect, which accounts for scattered radiation. A proportion of the beam crosses the patient, with part of its energy being absorbed (photoelectric effect) before reaching the detector. The differences in the amount of X-ray absorbed as it passes through the body results in variable attenuation and, therefore, heterogeneous intensity of the X-rays leaving the body. Production of radiological images is then this phenomenon.

The beam generated by X-ray machines is composed of X-rays carrying various energies (Figure A3). “Soft” X-rays carry low energy photons and are rapidly stopped by matter (absorption), they will mostly induce ionisation and are not useful for producing images.³ “Hard” X-rays with high energy photons cross biological matter with minimal interaction also does not generate a radiological image. The “intermediate” X-rays, however, carry enough energy to allow part of the beam to cross the matter and reach the detector and the rest to be absorbed. This is the fraction of the X-ray beam that will produce images.

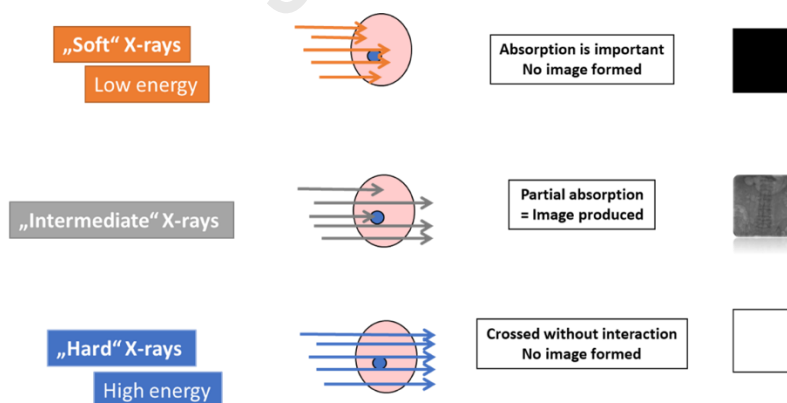


Figure A3: Differences between the X-rays produced in a generator and their role in producing an image.

Spectral filters, usually made of aluminium or copper, are positioned at the exit of the X-ray generator tube and used to stop or attenuate the low energy “soft” X-rays. Without this, the image generated by the X-ray machine would be blurred.

The filtered X-ray beam directed towards the body crosses structures that have different densities. Once the uniform X-rays enters the patient, the range of densities of the structures it crosses results in a range of attenuation, thus transforming it into a heterogenous beam,⁴ that is registered as a characteristic image via the detectors (Figure A4).

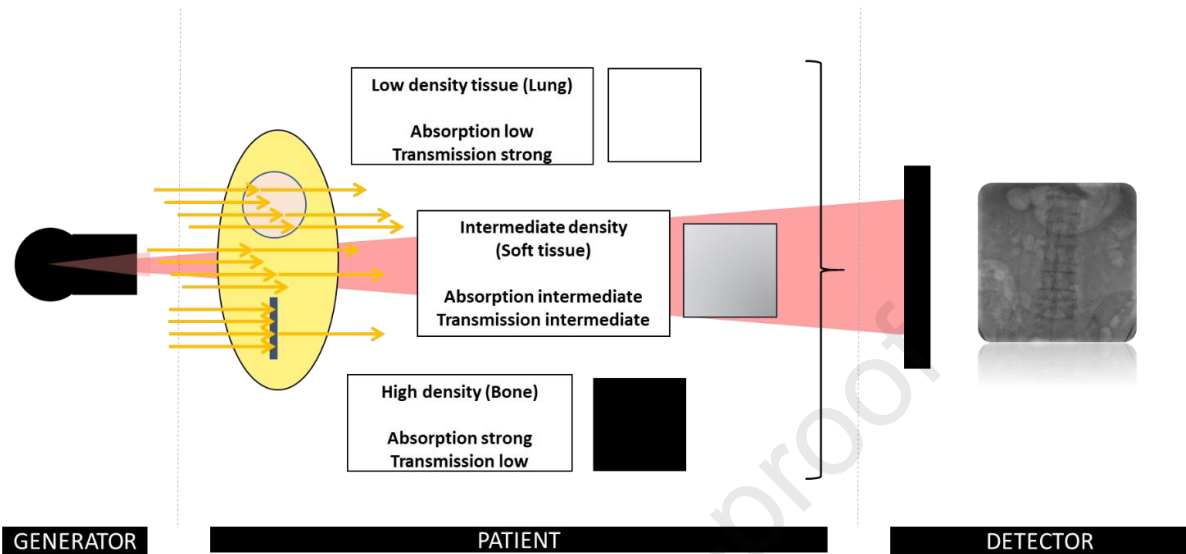


Figure A4: Image formation from the different densities of the structures crossed by the X-ray beam.

Appendix 2: Radiation exposures reported for endovascular procedures

Author	Year	Groups	Imaging System	Number of patients	KAP (Gy.cm ²)	CAK (mGy)	Dose to the operator (μSv)	Dose to the staff (μSv)
De Ruiter ⁵	2016		Mobile C-arm (Flat panel)	13	55.5 ± 38.9 (17.0–152.0)	300 ± 200 (100–600)	-	-
			Fixed C-arm	7	244.5 ± 142.2 (47.4–409.5)	820 ± 540 (100–1600)	-	-
			Fixed C-arm (Hybrid room)	26	157.0 ± 120.4 (25.9–418.0)	600 ± 400 (100–1600)	-	-
Antoniou ⁶	2016	EVAS	Mobile C-arm	32	54 (IQR 42.1–76.8)	.	-	-
		EVAR	Mobile C-arm	32	111 (IQR 75.3–157.4)	.	-	-
Machado ⁷	2016		Mobile C-arm	127	48 ± 32	.	-	-
Stansfield ⁸	2016	Without preprocedure run through and brief	Fixed C-arm	61	225.11 (16.63–1671.57)	-	-	-
		With preprocedure run through and brief	Fixed C-arm	44	142.22 (20.98–635.31)	-	-	-
Nyheim ⁹	2016		Fixed C-arm	80	234 (81–517)	-	-	-
Bacchi Neto ¹⁰	2016		Fixed C-arm	30	-	-	292.6 (88.4–459.5) ▯	207.0 (73.6–407.0) ▯
Dias ¹¹	2016	Standard dose protocol	Fixed C-arm	25	213.83 (IQR 123.99–290.14)*	-	-	-
		Low-dose protocol, Fusion imaging	Fixed C-arm	22	98.85 (IQR 83.63–164.70)*	-	-	-
Attigh ¹²	2016		Fixed C-arm (Hybrid room)	65	23 ± 25	-	620 ± 620†	470 ± 340†
El-Sayed ¹³	2017		Fixed C-arm	6	82.8 (53.61–144.3)	-	11 (4–74)	92 (43–203) ‡
Tuthill ¹⁴	2017	Centre 1	Fixed C-arm	74	77.96 ± 7.04	504.47 ± 55.07	-	-
		Centre 2		32	318.97 ± 57.97	1219.22 ± 296.48	-	-
		Centre 3		18	43.43 ± 9.94	218.09 ± 42.75	-	-

		Centre 4	Fixed C-arm (Hybrid room)	21	181.99 ± 21.41	983 ± 100.18	-	-
		Centre 5		35	114.23 ± 13.90	790.86 ± 118.11	-	-
Stangeberg¹⁵	2018		Fixed C-arm (Hybrid room)	25	-	581 (116.2-2695.8)*	-	-
			Fixed C-arm	52	-	1178.5 (174.9-3351.1)*	-	-
Miller¹⁶	2018	Baseline	Fixed C-arm	8	-	-	120 ± 70α	-
		Use of live dosimeters	Fixed C-arm	5	-	-	190 ± 40α	-
			Fixed C-arm (Hybrid room)	5	-	-	30 ± 20α	-
Ruffino¹⁷	2018		Fixed C-arm	25	337 (232-609)*	1608 (933-2770)*	-	-
			Fixed C-arm (Hybrid room)	25	157 (113-212)*	884 (558-1379)*	-	-
De Ruiter¹⁸	2018		Fixed C-arm (Hybrid room)	38	93.1 (63.5-132.5)*	400 (300-700)*	28α	16α
Schaefer¹⁹	2018		Fixed C-arm (Hybrid room)	53	168.34 ± 146.92	-	-	-
			Mobile C-arm (Flat panel)	107	49.93 (± 38.06)	-	-	-
Ahmad²⁰	2018	Without Fusion	Fixed C-arm (Hybrid room)	47	32.19 (IQR 14.31-49.42)*	-	-	-
		With Fusion	Fixed C-arm (Hybrid room)	105	23.44 (IQR 15.77-51.44)*	-	-	-
Hiraoka²¹	2018	Without Fusion	Fixed C-arm (Hybrid room)	62	-	880 ± 833	-	-
		With Fusion	Fixed C-arm (Hybrid room)	81	-	768 ± 529	-	-
Maurel²²	2018	Without cloud-based fusion (Cydar)	Fixed C-arm (Hybrid room)	21	21.7 (8.9-85.9)*	142 (61-541)*	-	-
		With cloud-based fusion (Cydar)	Fixed C-arm (Hybrid room)	33	9.17 (6.83-14.74)*	70 (45-100)*	-	-
Hertault²³	2018		Fixed C-arm (Hybrid room)	85	14.7 (IQR 10.0-27.7)*	107 (IQR 68.0-189.0)*	-	-
Ockert²⁴	2018	EVAR	Mobile C-arm (Flat panel)	30	22.6*	139*	-	-

		EVAS	Mobile C-arm (Flat panel)	30	12.4*	67.7*	-	-
<u>Tzanis</u> <u>25</u>	20 19		Not specified	17	124.3 (41.4-627.1)*		4.7±1.4α	
<u>Schulz</u> <u>26</u>	20 19		Fixed C-arm (Hybrid room)	50	96.6 (±90.3)			
<u>Kaladi</u> <u>i</u> ²⁷	20 19	With cloud-based fusion (Therenva)	Mobile C-arm (Flat panel)	49	70.9 (± 48.2)			
-		Without fusion (historical cohort)	Mobile C-arm (Flat panel)	103	67.3 (± 74)			
<u>Wermelink</u> ²⁸	20 19		Fixed C-arm (Hybrid room)	77	43.3* (IQR 28.4-63.3)		13 to 45α	
<u>Tenorio</u> <u>o</u> ²⁹	20 19		Fixed C-arm (Hybrid room)	24	105 (± 116)	373 (± 257)		
<u>Rehman</u> <u>n</u> ³⁰	20 20		Mobile C-arm	78	168 (± 111)			
			Fixed C-arm (Hybrid room)	208	82 (±75)			
<u>Väpenstad</u> ³¹	20 20	Patient specific rehearsal with virtual reality	Not specified	30	12* (2.9-50.9)			
		No rehearsal	Not specified	30	13* (3.4-31.5)			
<u>Zurche</u> <u>r</u> ³²	20 20	Standard imaging protocol	Fixed C-arm	17	174 (±79)	795.8 (±371.5)		
		Restricted use of angiography	Fixed C-arm	26	132 (±108)	761.4 (±721.4)		
<u>Tzanis</u> <u>33</u>	20 20		Fixed C-arm	73	153.2*			
<u>Harbrön</u> ³⁴	20 20		Fixed C-arm	81	75* (IQR 48-148)			
<u>Peters</u> ³⁵	20 20	EVAR	Fixed C-arm (Hybrid room)	40	278* (IQR 254-348)			

		EVAS	Fixed C-arm (Hybrid room)	67	275* (IQR 240-326)			
<u>Martin ez</u> ³⁶	20 20		Mobile C- arm	42	61.5 (±42.4)			
<u>Tanta wy</u> ³⁷	20 20	Using CO2 and CEUS	Not specified	15		182* (±135)		
<u>Rial</u> ³⁸	20 20		Mobile C- arm	165	80 (±58)	307 (±257)		
<u>Doelar e</u> ³⁹	20 20	Without Fusion	Fixed C-arm (Hybrid room)	41	139.8 (±186.8)	694.0 (±913.8)		
-		With Fusion		20	159.1 (±102.4)	810.7 (±496.7)		
<u>Farah</u> ⁴⁰	20 20			1 4 3	39.1 (0.1– 30.1)			
<u>Haga</u> ⁴¹	20 20		Fixed system	172	371.3 (± 186.0)	1101 (±540)		
<u>Kakko s</u> ⁴²	20 21		Mobile C- arm	48	26.8 (20.8- 38.1)			
<u>Efthv miou</u> ⁴³	20 21		Mobile C- arm	87	36.6* (2.0– 167.8)			

Table A1: Literature review of published dose reports after EVAR between 2016 and 2022. Results are reported in means with standard deviation (SD) or (*) in median with range, or interquartile range (IQR) if stated. ♂, Dose measurement above the lead protections; †, Dose to the anesthesiologists; ‡. ALARA : As Low As reasonable Achievable; KAP: Kerma-Area Product; CAK: Cumulative Air-kerma; CEUS: Contrast-Enhanced UltraSound; EVAR: Endovascular Aortic aneurysm Repair; EVAS: Endovascular Aortic aneurysm Sealing.

87
88
89
90
91
92

Author	Year	Groups	Imaging System	Number of patients	KAP (Gy.cm ²)	CAK (mGy)	Dose to the operator (μSv)	Dose to the staff (μSv)
Kirkwood ⁴⁴	2016		Fixed C-arm	16	601	4970	21.5	13.2
			Fixed C-arm (Hybrid room)	25	372	2580	14.1	7.1
De Ruiter ⁵	2016		Fixed C-arm	15	873.8 ± 652.5 (129.7–2590)	6000 ± 4700 (800 – 18000)	-	-
			Fixed C-arm (Hybrid room)	19	598.2 ± 318.5 (128.6–1362)	3700 ± 2500 (1000–10000)	-	-
Dias ¹¹	2016	Standard Dose protocol (FEVAR)	Fixed C-arm	36	283.24 (IQR 192.08–499.57)*	-	-	-
		Standard Dose protocol (BEVAR)	Fixed C-arm	23	638.91 (IQR 436.96–1002.66)*	-	-	-
		Low Dose protocol and Fusion imaging (BEVAR)	Fixed C-arm	21	241.72 (IQR 140.44–432.04)*	-	-	-
		Low Dose protocol and Fusion imaging (FEVAR)	Fixed C-arm	33	262.87 (IQR 202.98–367.69)*	-	-	-
Attigah ¹²	2016	FEVAR	Fixed C-arm (Hybrid room)	25	39 ± 33	-	1020 ± 1530†, 690 ± 460‡	-
		BEVAR	Fixed C-arm (Hybrid room)	17	48 ± 38	-	1310 ± 1580†, 700 ± 650‡	-
Wang ⁴⁵	2018	FEVAR	Fixed C-arm (Hybrid room)	91	-	4159 ± 2573	-	-
		Fenestrated cuff	Fixed C-arm (Hybrid room)	12	-	6063 ± 3086	-	-
De Ruiter ¹⁸	2018		Fixed C-arm (Hybrid room)	24	384.8 (265.2–522.3)*	2900 (2000–3700)*	297μ	171μ
Manunga ⁴⁶	2018		Fixed C-arm (Hybrid room)	84	-	1097 (IQR 978–1426)*	-	-

Rufino¹⁷	2018		Fixed C-arm	25	567 (388–779)*	2882 (2011–4230)*	-	-
Kirkwood⁴⁷	2018	FEVAR	Fixed C-arm (Hybrid room)	11	210*	1800*	120*α	60*α
		off the shelf FEVAR	Fixed C-arm (Hybrid room)	9	280*	2200*	220*α	110*α
		CMD	Fixed C-arm (Hybrid room)	60	370*	2950*	370*α	210*α
Schanzer⁴⁸	2020	FEVAR		732	82.8 (±158.9)	2920 (±2987)		
		Fenestrated cuff after failed EVAR		161	154.6 (±218.5)	4750 (±18,304)		
Harbrun³⁴	2020		Fixed C-arm	66	119* (IQR 85-209)			
Junjeja⁴⁹	2020		Mobile C-arm	11		2160 (±930.0)		
Timara⁵⁰	2020	With magnification	Fixed C-arm (Hybrid room)	123		2458* (IQR 1706-3767)	266* (IQR 104-583)α	
		With digital zoom	Fixed C-arm (Hybrid room)	28		1382* (IQR 999-2045)	101* (IQR 34-235)α	
Sen⁵¹	2020		Fixed C-arm (Hybrid room)	334	182 (±96)	2100 (±1800)		
Tenorio²⁹	2019		Fixed C-arm (Hybrid room)	85	174 (±101)	1134 (±815)		
Dolarel³²	2020		Fixed C-arm (Hybrid room)	37	91.5 (±348.4)	2337.2 (±1744.9)		

Table A2: Literature review of published dose reports after fenestrated or branched endovascular aortic aneurysm repair (F/BEVAR) between 2016 and 2022. Results are reported in means with standard deviation (SD) or (*) in median with range, or interquartile range (IQR) if stated. α, Dose measurement above the lead protections; ‡, Dose to the anesthesiologists. ALARA: As Low As reasonable Achievable; KAP: Kerma-Area Product; CAK: Cumulative Air-kerma.

Author	Year	Anatomical Regions	Procedures	Imaging System	Number of patients	KAP (Gy.cm ²)	CAK (mGy)	Dose to the operator (μSv)	Dose to the staff (μSv)
Ruiz-Cruces⁵²	2016	Iliac		Fixed C-arm	48	105.7			
		Femoro popliteal	Recanalization	Fixed C-arm	57	83.9			

Maurel ⁵³	2017	Iliac	Patients treated in 2012	Mobile & Fixed C-arm	653	14.2 (± 18.9)			
			Patients treated in 2015	Mobile & Fixed C-arm	306	21.5 (± 37.6)			
Stangenberg ¹⁵	2018	Femoro popliteal		Fixed C-arm	99		285.6* (IQR 152.7-486.8)		
				Fixed C-arm (Hybrid room)	35		106.0* (IQR 82.5-163.5)		
Kostova Lefterova ⁵⁴	2018	Femoro popliteal	PTA alone	Mobile C-arm	78	67* (0.6-711)			
			PTA + Stenting		20	78* (2.3-237)			
			Recanalization + PTA		39	75* (3.5-353)			
			Recanalization + stenting		52	121* (3.0-160)			
Guillou ⁵⁵	2018	Iliac	Serie n°1	Mobile C-arm	43	37.7	173.4		
			Serie n°1	Fixed C-arm	100	50	252.9		
		Femoro popliteal	Serie n°1	Mobile C-arm	56	21.5	93.8		
			Serie n°1	Fixed C-arm	99	20.2	98.1		
		Iliac & Femoro popliteal	Serie n°2	Mobile C-arm	24	19.4	66.6	0.2; 15.3	0.9
			Serie n°2	Fixed C-arm	76	24.2	125.8	0.3; 15.7	0.8
Goldswieg ⁵⁶	2019	Aortoiliac			3215	252.0 (±294.4)			
		Femoro popliteal			7203	145.6 (±212.2)			
Boc ⁵⁷	2019	Iliac	Angioplasty	Mobile C-arm	37	43.5* (IQR 28.6-87.4)			
			Stenting		161	54.9* (IQR 32.5-91.2)			
		Femoro popliteal	Angioplasty, antegrade approach		446	5.9* (IQR 4.3-8.6)			
			Angioplasty, retrograde approach		34	30.8* (IQR 22.2-48.3)			
			Stenting, antegrade approach		113	8.3* (IQR 6.0-12.3)			
			Stenting, retrograde approach		7	56.9* (20.0-93.7)			
Stahlberg ⁵⁸	2019	Iliac	With Fusion	Fixed C-arm	11	28.7* (IQR 19.7-42.2)			
			Without Fusion		15	43.8* (IQR 28.0-84.6)			

Tzanis ²⁵	20 19	Aortoiliac		Not specified	36	23.1* (37.0-296.0)		4.4±3.6 α	
Farah ⁴⁰	20 20	Iliac			130	14.4* (0.4-119.9)			
		Femoro popliteal			117	4.1* (0.1-146.8)			
Mougin ⁵⁹	20 22	Iliac		Fixed C-arm	56	14*; 21.52 (\pm 4.14)	237 (46)		
		Femoro popliteal			123	4*; 8.46 (\pm 1.60)	80 (14)		

Table A3: Literature review of published dose reports after endovascular repair of lower extremities arterial disease between 2016 and 2020. Results are reported in means with standard deviation (SD) or (*) in median with range, or interquartile range (IQR) if stated. α , Dose measurement above the lead protections. ALARA: As Low As reasonable Achievable; KAP: Kerma-Area Product; CAK: Cumulative Air-kerma.

References

- Hall E, Amato J. Giaccia, Radiobiology for the Radiologist, 6th edition. Philadelphia: Lippincott Williams & Wilkins, 2006.
- Bushberg JT. The Essential Physics of Medical Imaging. Philadelphia: Lippincott Williams & Wilkins, 2002.
- Russo P. Handbook of X-ray Imaging: Physics and Technology. CRC Press, 2017.
- Hendee WR, Ritenour ER. Medical Imaging Physics. John Wiley & Sons Inc; 2003.
- de Ruiter QMB, Moll FL, Gijsberts CM, van Herwaarden JA. AlluraClarity Radiation Dose-Reduction Technology in the Hybrid Operating Room During Endovascular Aneurysm Repair. Journal of Endovascular Therapy: An Official Journal of the International Society of Endovascular Specialists. 2016;23:130-8.
- Antoniou GA, Senior Y, Iazzolino L, England A, McWilliams RG, Fisher RK, et al. Endovascular Aneurysm Sealing Is Associated With Reduced Radiation Exposure and Procedure Time Compared With Standard Endovascular Aneurysm Repair. Journal of Endovascular Therapy: An Official Journal of the International Society of Endovascular Specialists. 2016;23:285-9.
- Machado R, Ferreira VMD, Loureiro L, Gonçalves J, Oliveira P, Almeida R. Radiation Exposure in Endovascular Infra-Renal Aortic Aneurysm Repair and Factors that Influence It. Brazilian Journal of Cardiovascular Surgery. 2016;31:415-21.
- Stansfield T, Parker R, Masson N, Lewis D. The Endovascular Preprocedural Run Through and Brief: A Simple Intervention to Reduce Radiation Dose and Contrast Load in Endovascular Aneurysm Repair. Vasc Endovascular Surg. 2016;50:241-6.
- Nyheim T, Staxrud LE, Jørgensen JJ, Jensen K, Olerud HM, Sandbæk G. Radiation exposure in patients treated with endovascular aneurysm repair: what is the risk of cancer, and can we justify treating younger patients? Acta Radiol. 2017;58:323-30.
- Bacchim Neto FA, Alves AF, Mascarenhas YM, Nicolucci P, Pina DR. Occupational radiation exposure in vascular interventional radiology: A complete evaluation of different body regions. Phys Med. 2016;32:1019-24.
- Dias NV, Billberg H, Sonesson B, Törnqvist P, Resch T, Kristmundsson T. The effects of combining fusion imaging, low-frequency pulsed fluoroscopy, and low-concentration contrast agent during endovascular aneurysm repair. J Vasc Surg. 2016;63:1147-55.

12. Attigah N, Oikonomou K, Hinz U, Knoch T, Demirel S, Verhoeven E, et al. Radiation exposure to eye lens and operator hands during endovascular procedures in hybrid operating rooms. *J Vasc Surg.* 2016;63:198-203.
13. El-Sayed T, Patel AS, Cho JS, Kelly JA, Ludwinski FE, Saha P, et al. Radiation-Induced DNA Damage in Operators Performing Endovascular Aortic Repair. *Circulation.* 2017;136:2406-16.
14. Tuthill E, O'Hora L, O'Donohoe M, Panci S, Gilligan P, Campion D, et al. Investigation of reference levels and radiation dose associated with abdominal EVAR (endovascular aneurysm repair) procedures across several European Centres. *Eur Radiol.* 2017;27:4846-56.
15. Stangenberg L, Shuja F, Bom IMJvd, Alfen MHGv, Hamdan AD, Wyers MC, et al. Modern Fixed Imaging Systems Reduce Radiation Exposure to Patients and Providers. *Vasc Endovascular Surg.* 2018;52:52-8.
16. Miller C, Kendrick D, Shevitz A, Kim A, Baele H, Jordan D, et al. Evaluating strategies for reducing scattered radiation in fixed-imaging hybrid operating suites. *J Vasc Surg.* 2018;67:1227-33.
17. Ruffino MA, Fronda M, Discalzi A, Isoardi P, Bergamasco L, Ropolo R, et al. Radiation dose during endovascular aneurysm repair (EVAR): upgrade of an angiographic system from standard to Eco mode. *Radiol Med.* 2018;123:966 -- 72.
18. de Ruiter QMB, Jansen MM, Moll FL, Hazenberg CEVB, Kahya NN, van Herwaarden JA. Procedure and step-based analysis of the occupational radiation dose during endovascular aneurysm repair in the hybrid operating room. *J Vasc Surg.* 2018;67:1881-90.
19. Schaefer JF, Wunderle K, Usai MV, Torsello GF, Panuccio G. Radiation doses for endovascular aortic repairs performed on mobile and fixed C-arm fluoroscopes and procedure phase-specific radiation distribution. *J Vasc Surg.* 2018;68:1889-96.
20. Ahmad W, Obeidi Y, Majd P, Brunkwall JS. The 2D-3D Registration Method in Image Fusion Is Accurate and Helps to Reduce the Used Contrast Medium, Radiation, and Procedural Time in Standard EVAR Procedures. *Ann Vasc Surg.* 2018;51:177-86.
21. Hiraoka A, Shiraya S, Chikazawa G, Ishida A, Miyake K, Sakaguchi T, et al. Feasibility of three-dimensional fusion imaging with multimodality roadmap system during endovascular aortic repair. *J Vasc Surg.* 2018;68:1175-82.
22. Maurel B, Martin-Gonzalez T, Chong D, Irwin A, Guimbretière G, Davis M, et al. A prospective observational trial of fusion imaging in infrarenal aneurysms. *J Vasc Surg.* 2018;68:1706-13.e1.
23. Hertault A, Rhee R, Antoniou GA, Adam D, Tonda H, Rousseau H, et al. Radiation Dose Reduction During EVAR: Results from a Prospective Multicentre Study (The REVAR Study). *Eur J Vasc Endovasc Surg.* 2018;56:426-33.
24. Ockert S, Heinrich M, Kaufmann T, Syburra T, Lopez R, Seelos R. Endovascular aortic sealing with Nellix reduces intraoperative radiation dose when compared to endovascular aortic repair. *J Vasc Surg.* 2018;67:1068-73.
25. Tzanis E, Tsetis D, Kehagias E, Ioannou CV, Damilakis J. Occupational exposure during endovascular aneurysm repair (EVAR) and aortoiliac percutaneous transluminal angioplasty (PTA) procedures. *Radiol Med.* 2019;124:539 -- 45.
26. Schulz CJ, Bockler D, Krisam J, Geisbusch P. Two-dimensional-three-dimensional registration for fusion imaging is noninferior to three-dimensional- three-dimensional registration in infrarenal endovascular aneurysm repair. *J Vasc Surg.* 2019;70:2005-13.
27. Kaladji A, Villena A, Pascot R, Lallys F, Daoudal A, Clochard E, et al. Fusion Imaging for EVAR with Mobile C-arm. *Ann Vasc Surg.* 2019;55:166-74.
28. Wermelink B, Willigendael EM, Smit C, Beuk RJ, Brusse-Keizer M, Meerwaldt R, et al. Radiation exposure in an endovascular aortic aneurysm repair program after introduction of a hybrid operating theater. *J Vasc Surg.* 2019;70:1927-34 e2.

29. Tenorio ER, Oderich GS, Sandri GA, Ozbek P, Karkkainen JM, Vrtiska T, et al. Prospective nonrandomized study to evaluate cone beam computed tomography for technical assessment of standard and complex endovascular aortic repair. *J Vasc Surg.* 2020;71:1982-93 e5.
30. Rehman ZU, Choksy S, Howard A, Carter J, Kyriakidis K, Elizabeth D, et al. Comparison of Patient Radiation Dose and Contrast Use during EVAR in a Dedicated Hybrid Vascular OR and Mobile Imaging. *Ann Vasc Surg.* 2019;61:278-83.
31. Vapenstad C, Lamoy SM, Aasgaard F, Manstad-Hulaas F, Aadahl P, Sovik E, et al. Influence of patient-specific rehearsal on operative metrics and technical success for endovascular aneurysm repair. *Minim Invasive Ther Allied Technol.* 2021;30:195-201.
32. Zurcher KS, Naidu SG, Money SR, Stone WM, Fowl RJ, Knuttinen G, et al. Dose reduction using digital fluoroscopy versus digital subtraction angiography in endovascular aneurysm repair: A prospective randomized trial. *J Vasc Surg.* 2020;72:1938-45.
33. Tzanis E, Ioannou CV, Tsetis D, Lioudaki S, Matthaïou N, Damilakis J. Complexity-based local diagnostic reference levels (DRLs) for standard endovascular aneurysm repair (EVAR) procedures. *Phys Med.* 2020;73:89-94.
34. Harbron RW, Abdelhalim M, Ainsbury EA, Eakins JS, Alam A, Lee C, et al. Patient radiation dose from x-ray guided endovascular aneurysm repair: a Monte Carlo approach using voxel phantoms and detailed exposure information. *J Radiol Prot.* 2020;40:704-26.
35. Peters AS, Hatzl J, Bischoff MS, Bockler D. Comparison of endovascular aneurysm sealing and repair with respect to contrast use and radiation in comparable patient cohorts. *J Cardiovasc Surg (Torino).* 2020;61:67-72.
36. Martinez LI, Esteban C, Riera C, Altes P, Llagostera S. Endovascular Infrarenal Aortic Aneurysm Repair Performed in a Hybrid Operating Room Versus Conventional Operating Room Using a C-Arm. *Ann Vasc Surg.* 2020;69:366-72.
37. Tantawy TG, Seriki D, Rogers S, Katsogridakis E, Ghosh J. Endovascular Aneurysm Repair Assisted by CO2 Digital Subtraction Angiography and Intraoperative Contrast-Enhanced Ultrasonography: Single-Center Experience. *Ann Vasc Surg.* 2021;70:459-66.
38. Rial R, Vañó E, Río-Solá MLD, Fernández JM, Sánchez RM, Santervás LAC, et al. National Diagnostic Reference Levels for Endovascular Aneurysm Repair and Optimisation Strategies. *Eur J Vasc Endovasc Surg.* 2020;60:837-42.
39. Doelare SAN, Smorenburg SPM, van Schaik TG, Blankensteijn JD, Wisselink W, Nederhoed JH, et al. Image Fusion During Standard and Complex Endovascular Aortic Repair, to Fuse or Not to Fuse? A Meta-analysis and Additional Data From a Single-Center Retrospective Cohort. *J Endovasc Ther.* 2021;28:78-92.
40. Farah J, Gonzalez-Mendez LA, Dufay F, Amir S, Royer B, Gabriel H, et al. Patient exposure and diagnostic reference levels in operating rooms: a multi-centric retrospective study in over 150 private and public French clinics. *J Radiol Prot.* 2020.
41. Haga Y, Chida K, Sota M, Kaga Y, Abe M, Inaba Y, et al. Hybrid Operating Room System for the Treatment of Thoracic and Abdominal Aortic Aneurysms: Evaluation of the Radiation Dose Received by Patients. *Diagnostics (Basel).* 2020;10.
42. Kakkos SK, Efthymiou FO, Metaxas VI, Dimitroukas CP, Panayiotakis GS. Factors affecting radiation exposure in endovascular repair of abdominal aortic aneurysms: a pilot study. *Int Angiol.* 2021;40:125-30.
43. Efthymiou FO, Metaxas VI, Dimitroukas CP, Kakkos SK, Panayiotakis GS. Kerma-Area Product, Entrance Surface Dose and Effective Dose in Abdominal Endovascular Aneurysm Repair. *Radiat Prot Dosimetry.* 2021;194:121-34.
44. Kirkwood ML, Guild JB, Arbique GM, Tsai S, Modrall JG, Anderson JA, et al. New image-processing and noise-reduction software reduces radiation dose during complex endovascular procedures. *J Vasc Surg.* 2016;64:1357-65.

45. Wang SK, Drucker NA, Sawchuk AP, Lemmon GW, Dalsing MC, Motaganahalli RL, et al. Use of the Zenith Fenestrated platform to rescue failing endovascular and open aortic reconstructions is safe and technically feasible. *J Vasc Surg.* 2018;68:1017-22.
46. Manunga J, Sullivan T, Garberich R, Alden P, Alexander J, Skeik N, et al. Single-center experience with complex abdominal aortic aneurysms treated by open or endovascular repair using fenestrated/branched endografts. *J Vasc Surg.* 2018;68:337-47.
47. Kirkwood ML, Chamseddin K, Arbique GM, Guild JB, Timaran D, Anderson JA, et al. Patient and operating room staff radiation dose during fenestrated/branched endovascular aneurysm repair using premanufactured devices. *J Vasc Surg.* 2018;68:1281 -- 6.
48. Schanzer A, Beck AW, Eagleton M, Farber MA, Oderich G, Schneider D, et al. Results of fenestrated and branched endovascular aortic aneurysm repair after failed infrarenal endovascular aortic aneurysm repair. *J Vasc Surg.* 2020;72:849-58.
49. Juneja A, Zia S, Ayad MH, Singh K, Dietch J, Schor J. Safety and Feasibility of Performing Fenestrated Endovascular Abdominal Aneurysm Repair Using a Portable C-arm Without Fusion Technology: A Single-Center Experience. *Cureus.* 2020;12:e7739.
50. Timaran LI, Timaran CH, Scott CK, Soto-Gonzalez M, Timaran-Montenegro DE, Guild JB, et al. Dual fluoroscopy with live-image digital zooming significantly reduces patient and operating staff radiation during fenestrated-branched endovascular aortic aneurysm repair. *J Vasc Surg.* 2021;73:601-7.
51. Sen I, Tenorio ER, Pitcher G, Mix D, Marcondes GB, Lima GBB, et al. Effect of obesity on radiation exposure, quality of life scores, and outcomes of fenestrated-branched endovascular aortic repair of pararenal and thoracoabdominal aortic aneurysms. *J Vasc Surg.* 2021;73:1156-66 e2.
52. Ruiz-Cruces R, Vano E, Carrera-Magarino F, Moreno-Rodriguez F, Soler-Cantos MM, Canis-Lopez M, et al. Diagnostic reference levels and complexity indices in interventional radiology: a national programme. *Eur Radiol.* 2016;26:4268-76.
53. Maurel B, Hertault A, Mont LSd, Cazaban S, Rinckenbach S. A Multicenter Survey of Endovascular Theatre Equipment and Radiation Exposure in France during Iliac Procedures. *Ann Vasc Surg.* 2017;40:50-6.
54. Kostova-Lefterova DD, Nikolov NN, Stanev SS, Stoyanova BB. Patient doses in endovascular and hybrid revascularization of the lower extremities. *Br J Radiol.* 2018;91:20180176.
55. Guillou M, Maurel B, Necib H, Vent P-A, Costargent A, Chaillou P, et al. Comparison of Radiation Exposure during Endovascular Treatment of Peripheral Arterial Disease with Flat-Panel Detectors on Mobile C-arm versus Fixed Systems. *Ann Vasc Surg.* 2018;47:104-13.
56. Goldsweig AM, Kennedy KF, Abbott JD, Jones WS, Velagapudi P, Rutar FJ, et al. Patient Radiation Dosage During Lower Extremity Endovascular Intervention. *JACC Cardiovasc Interv.* 2019;12:473-80.
57. Boc V, Boc A, Zdesar U, Blinc A. Patients' radiation doses during percutaneous endovascular procedures in arteries of the lower limbs. *Vasa.* 2019;48:167-74.
58. Stahlberg E, Sieren M, Anton S, Jacob F, Planert M, Barkhausen J, et al. Fusion Imaging Reduces Radiation and Contrast Medium Exposure During Endovascular Revascularization of Iliac Steno-Occlusive Disease. *Cardiovasc Intervent Radiol.* 2019;42:1635-43.
59. Mougin J, Louis N, Maupas E, Goueffic Y, Fabre D, Haulon S. Fusion imaging guidance for endovascular recanalization of peripheral occlusive disease. *J Vasc Surg.* 2022;75:610-7.

European Society for Vascular Surgery (ESVS) 2023 Clinical Practice Guidelines on Radiation Safety

Writing Committee:

Bijan Modarai, Professor of Vascular Surgery and British Heart Foundation Senior Fellow, Academic Department of Vascular Surgery, School of Cardiovascular and Metabolic Medicine and Sciences, BHF Centre of Excellence and the Biomedical Research Centre at Guy's & St Thomas' NHS Foundation Trust and King's College London, United Kingdom (chair)

Stéphan Haulon, Professor of Vascular and Endovascular Surgery, Aortic Center, Hôpital Marie Lannelongue, Groupe Hospitalier Paris St Joseph, Université Paris Saclay, France (co-chair)

Adrien Hertault, Vascular and Endovascular Surgeon, Department of Vascular Surgery, Ramsay Santé, Hôpital Privé de Villeneuve d'Ascq, France

Anders Wanhainen, Professor of Vascular Surgery, Department of Surgical Sciences, Uppsala University, Uppsala, Sweden and Guest Professor of Surgery, Department of Surgical and Perioperative Sciences, Surgery, Umeå University, Sweden

Ashish Patel, Senior Lecturer in Vascular Surgery and Honorary Consultant Vascular Surgeon, Academic Department of Vascular Surgery, School of Cardiovascular and Metabolic Medicine and Sciences, BHF Centre of Excellence and the Biomedical Research Centre at Guy's & St Thomas' NHS Foundation Trust and King's College London, United Kingdom

Dittmar Böckler, Professor of Vascular and Endovascular Surgery, University Hospital Heidelberg, 69120 Heidelberg, Germany

Eliseo Vano, Emeritus Professor of Medical Physics, Radiology Department. Medicine School, Complutense University, 28040 Madrid, Spain

Elizabeth Ainsbury, Cytogenetics Group Leader, UK Health Security Agency Radiation, Chemical and Environmental Hazards Division (UKHSA RCEHD), Chilton, Didcot, Oxon OX11 0RQ, UK and Environmental Research Group within the School of Public Health, Faculty of Medicine at Imperial College of Science, Technology and Medicine, London, UK

Isabelle Van Herzele, Associate Professor of Vascular Surgery, Department of Thoracic and Vascular Surgery, Ghent University Hospital, Ghent, Belgium

Joost van Herwaarden, Professor of Vascular Surgery, Department of Vascular Surgery, University Medical Center Utrecht, Utrecht, The Netherlands

Joseph Dawson, Consultant Vascular and Endovascular Surgeon, Royal Adelaide Hospital and Associate Professor, University of Adelaide, South Australia, Australia

Mark Farber, Chief, Division of Vascular Surgery, Director, UNC Aortic Network, Professor of Surgery and Radiology, Department of Surgery, University of North Carolina, Chapel Hill, NC, USA

Salome Weiss, Consultant Vascular Surgeon, Department of Vascular Surgery, Inselspital, Bern University Hospital, University of Bern, Switzerland

ESVS Guidelines Committee:

Frederico Bastos Gonçalves, Centro Hospitalar Universitário de Lisboa Central & NOVA Medical School, Lisbon, Portugal

Martin Björck, Department of Surgical Sciences, Vascular Surgery, Uppsala University, Uppsala, Sweden
Department of Surgery, Institute of Clinical Medicine, University of Tartu, Tartu, Estonia

Nabil Chakfé, University of Strasbourg, Strasbourg, France

Gert J. de Borst, Department of Vascular Surgery, university medical center utrecht, Utrecht, The Netherlands

Raphaël Coscas, Ambroise Paré University Hospital, AP-HP, Boulogne-Billancourt, Versailles-Saint-Quentin and Paris-Saclay Universities, France

Nuno V. Dias, Vascular Center, Department of Thoracic and Vascular Surgery, Skåne University Hospital, Malmö, Sweden and Department of Clinical Sciences Malmö, Lund University, Malmö, Sweden

Florian Dick, Department of Vascular Surgery, Kantonsspital St. Gallen, and University of Berne, Berne, Switzerland

Robert J. Hinchliffe, Department of Vascular Surgery, University of Bristol, Bristol, UK

Stavros K. Kakkos, Department of Vascular Surgery, University of Patras Medical School, Patras, Greece

Philippe Kolh, Department of Biomedical and Preclinical Sciences, University of Liège, and GIGA Cardiovascular Sciences, University of Liège, Liège, Belgium

Igor B. Koncar, Faculty of Medicine, University of Belgrade, Belgrade, Serbia

Jes S. Lindholt, Department of Cardiothoracic and Vascular surgery, Odense University Hospital and Elite research centre of individualised medicine for arterial disease (CIMA), Odense University Hospital, Odense, Denmark

Santi Trimarchi, Fondazione IRCCS Cà Granda Ospedale Maggiore Policlinico Milan, Milan, Italy - Department of Clinical and Community Sciences, University of Milan, Milan, Italy

Riikka Tulamo, Helsinki University Hospital and University of Helsinki, Helsinki, Finland

Christopher P. Twine, North Bristol NHS Trust, Bristol, UK University of Bristol, Bristol, UK

Frank Vermassen, Department of Vascular and Thoracic Surgery; Ghent University Hospital. Ghent, Belgium (review coordinator)

Document Reviewers:

Klaus Bacher, Medical physics, Ghent University, Ghent, Belgium

Elias Brountzos, Interventional Radiology, National and Kapodistrian University of Athens, Athens, Greece

Fabrizio Fanelli, Careggi University Hospital, Florence, Italy

Liliana A. Fidalgo Domingos, Centro Hospitalar Universitario do Algarve, Faro, Portugal

Mauro Gargiulo, Vascular Surgery, DIMES, University of Bologna, IRCCS Policlinico S. Orsola, Bologna Italy

Kevin Mani, Department of surgical sciences, Uppsala university, Uppsala, Sweden

Tara M. Mastracci, St. Bartholomew's Hospital, London, UK

Blandine Maurel, CHU, Nantes, France.

Robert A. Morgan, St George's University Hospitals NHS Foundation Trust & St George's University of London

Peter Schneider, Vascular and Endovascular Surgery, University of California San Francisco, San Francisco, USA

ADDITIONAL DETAILS FROM THE JOURNAL MANAGER.

- *Please ensure that the formatting for this paper follows YEJVS_8370.**
- *Please see list of files below. Note the three that are to be used to create the S5.**
- *The following other files will be sent for copy editing.**
- *There are 17 graphics and 2 e-comp files.**
- *Please check YEJVS_8370 and copy the tagging and listing for the ESVS Guidelines Committee / Document Reviewers.**

Guidelines def version clean_for preproof clean 140922 – USE TO CREATE S5

Appendix Affiliations Radiation Safety 2022_for preproof – USE TO CREATE S5

Appendix 1 and 2 def clean(1)_for preproofs – USE TO CREATE S5

Comments for copy editors and typesetters 140922_DO NOT USE FOR PRE PROOF

Guidelines def version_clean 140922_DO NOT USE FOR PRE PROOF

Radiation safety gl Style ed Tables 300822_lang_DO NOT USE FOR PRE PROOF

Radiation safety gl Style ed Fig legends 300822_lang_DO NOT USE FOR PRE PROOF

Appendix Affiliations Radiation Safety 2022_DO NOT USE FOR PRE PROOF

Appendix 1 and 2 def clean(1)_DO NOT USE FOR PREPROOFS